


HP 85031B 7 mm CALIBRATION KIT



Printed: MARCH 1986

© Copyright HEWLETT-PACKARD COMPANY 1986
1400 FOUNTAINGROVE PARKWAY, SANTA ROSA, CALIFORNIA, 95401, U.S.A.

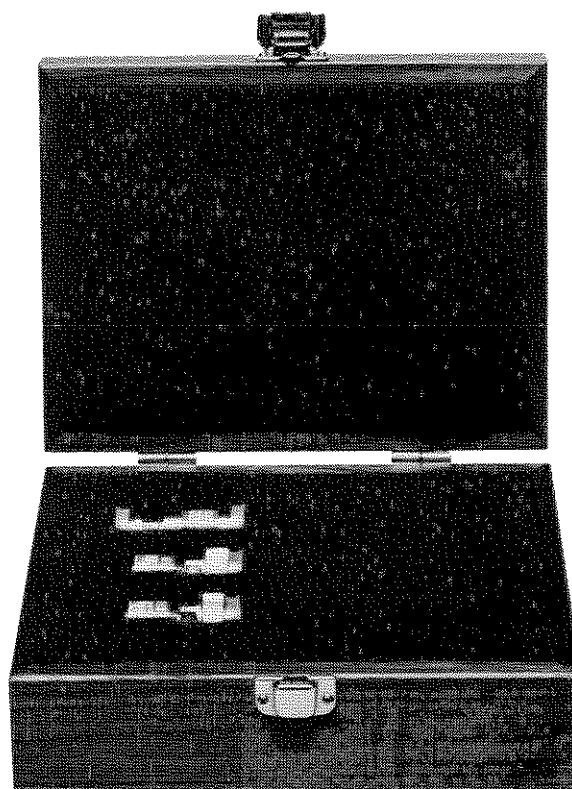

**HEWLETT
PACKARD**

WARRANTY

This Hewlett-Packard instrument product is warranted against defects in material and workmanship for a period of one year from date of delivery. During the warranty period, Hewlett-Packard Company will, at its option, either repair or replace products which prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by HP. Buyer shall prepay shipping charges to HP and HP shall pay shipping charges to return the product to Buyer. However, Buyer shall pay all shipping charges, duties, and taxes for products returned to HP from another country.

HP warrants that its software and firmware designated by HP for use with an instrument will execute its programming instructions when properly installed on that instrument. HP does not warrant that the operation of the instrument, or software, or firmware will be uninterrupted or error free.

LIMITATION OF WARRANTY

The foregoing warranty shall not apply to defects resulting from improper handling by Buyer, Buyer-supplied software or interfacing, unauthorized modification or misuse, or operation outside of the environmental specifications for the product.

NO OTHER WARRANTY IS EXPRESSED OR IMPLIED, HP SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OR MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

EXCLUSIVE REMEDIES

THE REMEDIES PROVIDED HEREIN ARE BUYER'S SOLE AND EXCLUSIVE REMEDIES, HP SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER BASED ON CONTRACT, TORT, OR ANY OTHER LEGAL THEORY.

ASSISTANCE


Product maintenance agreements and other customer assistance agreements are available for Hewlett-Packard Products.

For any assistance, contact your nearest Hewlett-Packard Sales and Service Office. Addresses are provided at the back of this manual.

GENERAL INFORMATION

To obtain optimum performance from this calibration kit, observe these simple precautions:

- Make connections carefully to avoid misalignment and connector damage or inaccurate measurements.
- Keep the connectors free of dirt and metallic particles.
- If you must clean the connectors, try clean compressed air first. Do not use abrasives. With a plastic swab, apply **only** liquid Freon (trichlorotrifluoroethane) as a solvent.
- For more information, refer to the Microwave Connector Care manual (HP part number 08510-90064) or application note 326, Principles of Microwave Connector Care (literature number 5954-1566).
- 7mm center conductor recession with collet removed: 0.0 to 0.002 inch.
- 7mm open collet compressor recession: 0.0 to 0.001 inch.

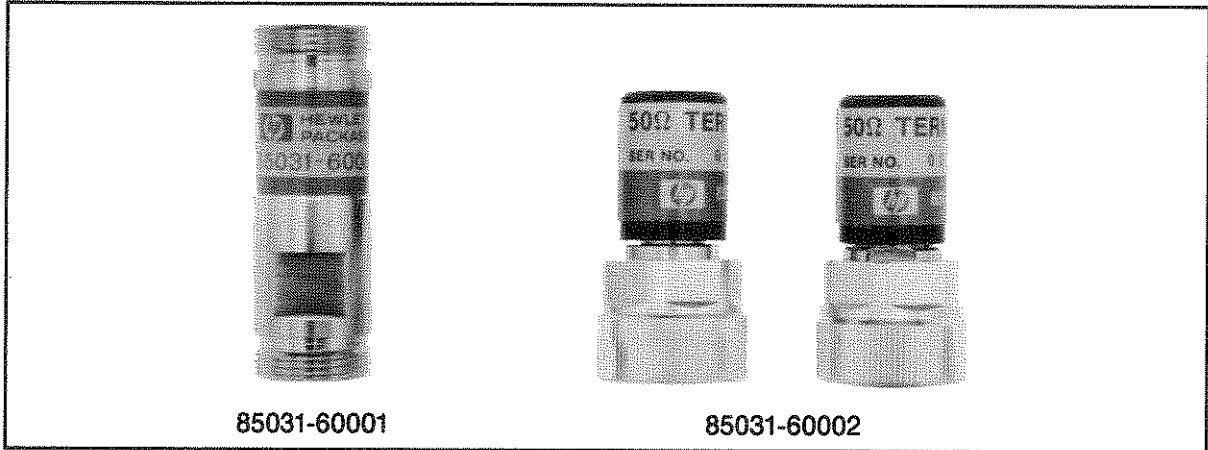

DESCRIPTION

The HP 85031B 7 mm calibration kit, illustrated above, contains precision standard devices designed to characterize the systematic errors of 7 mm measurement systems. The storage case is supplied to protect the calibration devices from damage that will degrade performance accuracy. Replace the devices in the case immediately after use. The kit's contents and characteristics are listed below.

CONTENTS

Qty	Description (Characteristic)	HP Part or Model Number
1	7 mm 50Ω combination open/short	85031-60001
2	7 mm 50Ω termination (return loss \geq 52 dB, DC to 3.0 GHz)*	85031-60002
1	HP 85031B Operating and Service Manual	85031-90003
1	storage case	85031-80002
1	storage case pad	85031-80003

*at 25° ± 5°C; typical resistance change is ±130ppm/°C

WEIGHT

Net	1.1 kg (2.4 lb)
Shipping	1.6 kg (3.5 lb)

STANDARD DEFINITIONS

STANDARD		C0 $\times 10^{-15}F$	C1 $\times 10^{-27}F/Hz$	C2 $\times 10^{-36}F/Hz$	C3 $\times 10^{-45}F/Hz$	FIXED OR SLIDING	OFFSET			FREQUENCY (GHz)		COAX or WAVEGUIDE	STANDARD LABEL
NO.	TYPE						DELAY ps	LOSS MΩ/s	Z ₀ Ω	MINIMUM	MAXIMUM		
1	SHORT						0	700	50	0	999	COAX	SHORT
2	OPEN	92.85	0	7.2	4.3		0	700	50	0	999	COAX	OPEN
3	LOAD					FIXED	0	700	50	0	999	COAX	BROAD- BAND
4	DELAY/ THRU						0	700	50	0	999	COAX	THRU
5													
6													
7													
8													

STANDARD CLASS ASSIGNMENTS

	A	B	C	D	E	F	G	STANDARD CLASS LABEL
S _{11A}	2							OPEN
S _{11B}	1							SHORT
S _{11C}	3							LOAD
S _{22A}	2							OPEN
S _{22B}	1							SHORT
S _{22C}	3							LOAD
Forward Transmission	4							THRU
Reverse Transmission	4							THRU
Forward Match	4							THRU
Reverse Match	4							THRU
Response	1	2	4					RESPONSE
Response & Isolation	1	2	4					RESPONSE & ISOL'N

The two tables on this page list the characteristics (standard definitions and standard class assignments) of the devices in this calibration kit. The information in these tables also resides in EEPROM in the HP 8753A. Use these tables with the calibration procedure described in the "Operating and Programming Reference" section of the HP 8753A manual.



For more information, call your local HP sales office listed in the telephone directory white pages. Ask for the Electronic Instruments Department. Or write to Hewlett-Packard: **U.S.A.** - P. O. Box 10301, Palo Alto, CA 94303-0690. **Europe** - P.O. Box 999, 1180 AZ Amstelveen, The Netherlands. **Canada** - 6877 Goreway Drive, Mississauga L4V 1M8, Ontario. **Japan** - Yokogawa-Hewlett-Packard Ltd., 3-29-21, Takaido-Higashi, Suginami-ku, Tokyo 168. **Elsewhere** in the world, write to Hewlett-Packard Intercontinental, 3495 Deer Creek Road, Palo Alto, CA 94304.

MANUAL PART NO. 85031-90003

Microfiche Part No. 85031-90004

Printed in U.S.A.