

Keysight X-Series Signal Analyzers

This manual provides documentation for the following analyzers:

PXA Signal Analyzer N9030A

MXA Signal Analyzer N9020A

EXA Signal Analyzer N9010A

CXA Signal Analyzer N9000A

Notice: This document contains references to Agilent. Please note that Agilent's Test and Measurement business has become Keysight Technologies. For more information, go to www.keysight.com.

Notices

© Keysight Technologies 2009-2014

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies, as governed by United States and international copyright laws.

Manual Part Number

N9020-90124

Print Date

August 2014

Supersedes: March 2014

Printed in USA

Keysight Technologies
1400 Fountaingrove Parkway
Santa Rosa, CA 95403

Warranty

The material contained in this document is provided “as is,” and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Keysight disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Keysight shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Keysight and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as “Commercial computer software” as defined in DFAR 252.227-7014 (June 1995), or as a “commercial item” as defined in FAR 2.101(a) or as

“Restricted computer software” as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Keysight Technologies’ standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

Where to Find the Latest Information

Documentation is updated periodically. For the latest information about these products, including instrument software upgrades, application information, and product information, see the following URLs:

<http://www.keysight.com/find/pxa>

<http://www.keysight.com/find/mxa>

<http://www.keysight.com/find/exa>

<http://www.keysight.com/find/cxa>

To receive the latest updates by email, subscribe to Keysight Email Updates:

<http://www.keysight.com/find/emailupdates>

Information on preventing instrument damage can be found at:

<http://www.keysight.com/find/PreventingInstrumentRepair>

Is your product software up-to-date?

Periodically, Keysight releases software updates to fix known defects and incorporate product enhancements. To search for software updates for your product, go to the Keysight Technical Support website at:

<http://www.keysight.com/find/techsupport>

Table of Contents

1 Contacting Keysight Sales and Service Offices	
2 Products Covered by this Document	
X-Series Processor and Disk Drive Configurations	10
Processor Assembly Configuration	10
Disk Drive Configuration	10
Determining Instrument Configuration based on Product Name	12
Processor Assembly Configuration	12
Disk Drive Configuration	13
Rear Panel Configurations	14
Determining Installed Options	15
3 Security Terms and Definitions	
4 Instrument Memory & Volatility	
Non-Volatile Memory	20
Disk Drive Partitioning	26
Volatile Memory	27
5 Memory Clearing, Sanitization and Removal Procedures	
Instrument Sanitization Procedures	31
Application License Key Storage	31
Regenerating a Site Key License for 89601A VSA Application	31
Replacement of Processor Assembly	31
Replacement of Disk Drive	33
Archiving and Restoring Factory Calibration Data Files	35
Tools Required	35
Determining Instrument Software Revision	36
Software Revision A.01.55 or Lower	37
Data Backup using XML File	37
Data Restore using XML File	37
Software Revision Greater than A.01.55 and Lower than A.02.00	37
Data Backup using Utility Program	38
Data Restore using Utility Program	38
Software Revision A.02.00 or Greater	39
Data Backup or Restore using Alignment Data Wizard	39
6 Processor Assembly Removal Procedure	
7 Disk Drive Removal Procedure	

Contents

Instruments with Non-Removable Drives	44
Instruments with Removable Drives	45
8 User and Remote Interface Security Measures	
SCPI/GPIB Control of Interfaces	47
Operating System Security Features	47
Determining the Instrument's Operating System	48
USB Interfaces	48
Disabling or Enabling AutoRun/AutoPlay	48
Windows 7	48
Windows XP	48
Configuring USB for Read-only	51
9 Procedure for Declassifying a Faulty Instrument	
10 Special Options	
Option SF1	56
Support	56
Menu & Command Changes	56
File Menu	56
System Menu	56
SCPI Commands	56
Right-Click (Popup) Menu	56
Option SF2	57
Support	57
Operating System Changes	57
Menu & Command Changes	58
Front-panel Keys	58
File Menu	58
System Menu	58
SCPI Commands	58
Right-Click (Popup) Menu	61
Appendix A References	

1 Contacting Keysight Sales and Service Offices

Assistance with test and measurement needs, and information to help you find a local Keysight office, is available via the internet at, <http://www.keysight.com/find/assist>. If you do not have internet access, please contact your designated Keysight representative.

NOTE

In any correspondence or telephone conversation, refer to the instrument by its model number and full serial number. With this information, the Keysight representative can determine whether your unit is still within its warranty period.

Contacting Keysight Sales and Service Offices

2 Products Covered by this Document

Product Family Name	Product Names	Model Numbers
X-Series Signal Analyzers	PXA Signal Analyzer	N9030A-503, -508, -513, -526, -543, -544, -550
	MXA Signal Analyzer	N9020A-503, -508, -513, -526
	EXA Signal Analyzer	N9010A-503, -507, -513, -526, -532, -544
	CXA Signal Analyzer	N9000A-503, -507, 513, -526

This document describes instrument memory types and security features. It provides a statement regarding the volatility of all memory types, and specifies the steps required to declassify an instrument through memory clearing, sanitization, or removal.

For additional information, go to:

<http://www.keysight.com/find/security>

IMPORTANT

Be sure that all information stored by the user in the instrument that needs to be saved is properly backed up before attempting to clear any of the instrument memory. Keysight Technologies cannot be held responsible for any lost files or data resulting from the clearing of memory.

Be sure to read this document entirely before proceeding with any file deletion or memory clearing.

X-Series Processor and Disk Drive Configurations

This document describes alternative Processor and Disk Drive Configurations for X-Series analyzers. Due to continuous improvement of the X Series Analyzer range, configurations may vary according to such factors as: manufacturing date, product name, and installed options. Processor and disk drive configurations are considered separately, due to the large number of possible combinations.

Processor Assembly Configuration

There are three possible processor assembly configurations: a single-core microprocessor with non-removable (fixed) disk drive, a single-core microprocessor with removable disk drive, or a dual-core processor with removable disk drive. The relationship between processor assembly type and product name is detailed in [Table 2-1](#) below. (For details of how to determine installed options, see [“Determining Installed Options” on page 15](#))

Table 2-1 Processor Assembly & Product Name

Type	Configuration	Product Names & Installed Options
1	Single-Core, Fixed Disk	<p>The disk is referred to as "fixed", because it can only be removed by removing and opening the instrument's processor assembly.</p> <p>This configuration is standard for:</p> <ul style="list-style-type: none"> a. MXA instruments without Option PC2 or PC4, b. EXA instruments without Option PC2, PC3, PC4 or PC5, c. CXA instruments without Option PC3 or PC5.
2	Single-Core, Removable Disk	<p>The disk may be removed from the instrument's rear panel, without removing or opening the processor assembly.</p> <p>This configuration is standard for:</p> <ul style="list-style-type: none"> a. EXA instruments with Option PC3 or PC5, b. CXA instruments with Option PC3 or PC5.
3	Dual-Core, Removable Disk	<p>The disk may be removed from the instrument's rear panel, without removing or opening the processor assembly.</p> <p>The Dual-Core processor unit is standard for:</p> <ul style="list-style-type: none"> a. all PXA instruments, b. MXA instruments with Option PC2 or PC4, c. EXA instruments with Option PC2 or PC4.

Disk Drive Configuration

There are several possible disk drive configurations, as listed below in [Table 2-2](#). The actual configuration depends on the instrument's Product Name and installed options (Options SSD, PC2, PC3, PC4 or PC5). For details of how to determine installed options, see [“Determining Installed Options” on page 15](#).

Products Covered by this Document
X-Series Processor and Disk Drive Configurations

For details of the capacities of each of the drive types listed below, see [“Non-Volatile Memory” on page 20](#).

Table 2-2 Disk Drive Configurations

Type	Configuration	Product Names & Installed Options
Fixed Magnetic	Fixed Magnetic Drive	This configuration applies to: <ol style="list-style-type: none"> a. MXA instruments without Option PC2 or PC4, b. EXA instruments without Option PC2, PC3, PC4 or PC5, c. CXA instruments without Option PC3 or PC5.
Removable Magnetic	Standard Removable Magnetic Drive	This configuration applies to: <ol style="list-style-type: none"> a. PXA instruments without Option SSD, b. MXA instruments with Option PC2, but without Option SSD. c. EXA instruments with Option PC2 or PC3, but without Option SSD. <p>(To determine whether your instrument includes Option SSD, which is now included with new instruments by default, see “Determining Installed Options” on page 15.)</p>
Removable Solid-State	Removable Solid-State Drive (Flash drive)	This configuration applies to all instruments with Option SSD , Option PC4 or Option PC5. Originally an option, a solid-state disk drive cartridge is now supplied by default with X-Series Analyzers.

Option SSD

You can obtain a **Removable Solid-State** disk drive for your instrument, either as an upgrade to replace a **Removable Magnetic** disk drive, or as an additional solid-state drive, by ordering Option SSD. You can order Option SSD either at the time that you purchase the instrument, or at any later time.

If your instrument’s current processor assembly configuration is **Single-Core, Fixed Disk**, in order to be able to use the removable disk you will need to upgrade the instrument to a **Dual-Core, Removable Disk** or **Single-Core, Removable Disk** processor assembly, by ordering Option PC4 or PC5 respectively. (Older CXA instruments may require Option PC3 instead of PC5. Before ordering, check with your Keysight Sales office, as described in [“Contacting Keysight Sales and Service Offices” on page 7](#).)

Note that **Removable Solid-State** disk units exist in **two** capacities. Earlier disks had a total capacity of 32 GB, while newer units have a total capacity of 80 GB.

Products Covered by this Document

Determining Instrument Configuration based on Product Name

Determining Instrument Configuration based on Product Name

Use the following procedures to determine the processor assembly and disk drive configurations of your instrument, starting from its Product Name.

Processor Assembly Configuration

The following procedure allows you to determine whether your instrument has a **Single-Core, Fixed Disk**, **Single-Core, Removable Disk** or **Dual-Core, Removable Disk** processor assembly.

Step	Procedure
1	What is the Product Name of your instrument? PXA: Go to Step 8. MXA: Go to Step 2. EXA: Go to Step 3. CXA: Go to Step 5.
2	Examine the instrument's rear panel and compare with the illustrations in "Rear Panel Configurations" on page 14. Does it resemble or Figure 2-1 (Fixed Disk) or Figure 2-2 (Removable Disk)? Fixed Disk: Go to Step 6. Removable Disk: Go to Step 8.
3	Examine the instrument's rear panel and compare with the illustrations in "Rear Panel Configurations" on page 14. Does it resemble or Figure 2-1 (Fixed Disk) or Figure 2-2 (Removable Disk)? Fixed Disk: Go to Step 6. Removable Disk: Go to Step 4.
4	Are Options PC2, PC3, PC4 or PC5 installed? (To determine whether any of these options are installed, see "Determining Installed Options" on page 15 below.) PC2 or PC4 installed: Go to Step 8. PC3 or PC5 installed: Go to Step 7.
5	Examine the instrument's rear panel and compare with the illustrations in "Rear Panel Configurations" on page 14. Does it resemble or Figure 2-1 (Fixed Disk) or Figure 2-2 (Removable Disk)? Fixed Disk: Go to Step 6. Removable Disk: Go to Step 7.
6	Your instrument has a Single-Core, Fixed Disk processor assembly.
7	Your instrument has a Single-Core, Removable Disk processor assembly.
8	Your instrument has a Dual-Core, Removable Disk processor assembly.

Disk Drive Configuration

The following procedure allows you to determine your instrument's disk drive configuration

Step	Procedure
1	What is the Product Name of your instrument? PXA: Go to Step 5. MXA: Go to Step 3. EXA: Go to Step 3. CXA: Go to Step 2.
2	Examine the instrument's rear panel and compare with the illustrations in "Rear Panel Configurations" on page 14. Does it resemble or Figure 2-1 (Fixed Disk) or Figure 2-2 (Removable Disk)? Fixed Disk: Go to Step 4. Removable Disk: Go to Step 6.
3	Examine the instrument's rear panel and compare with the illustrations in "Rear Panel Configurations" on page 14. Does it resemble or Figure 2-1 (Fixed Disk) or Figure 2-2 (Removable Disk)? Fixed Disk: Go to Step 4. Removable Disk: Go to Step 5.
4	Your instrument has a 40 GB Fixed Magnetic disk drive.
5	Check the instrument's installed options (see "Determining Installed Options" on page 15). If the list includes "N90X0A-IDE", your instrument has a 160 GB Removable Magnetic disk drive. If the list includes "N90X0A-SSD", your instrument has a 32 GB or 80 GB Removable Solid-State disk drive.
6	Your instrument has a 32 GB or 80 GB Removable Solid-State disk drive.

Products Covered by this Document
Determining Instrument Configuration based on Product Name

Rear Panel Configurations

Figure 2-1 Rear Panel of Instrument with Fixed Magnetic Disk


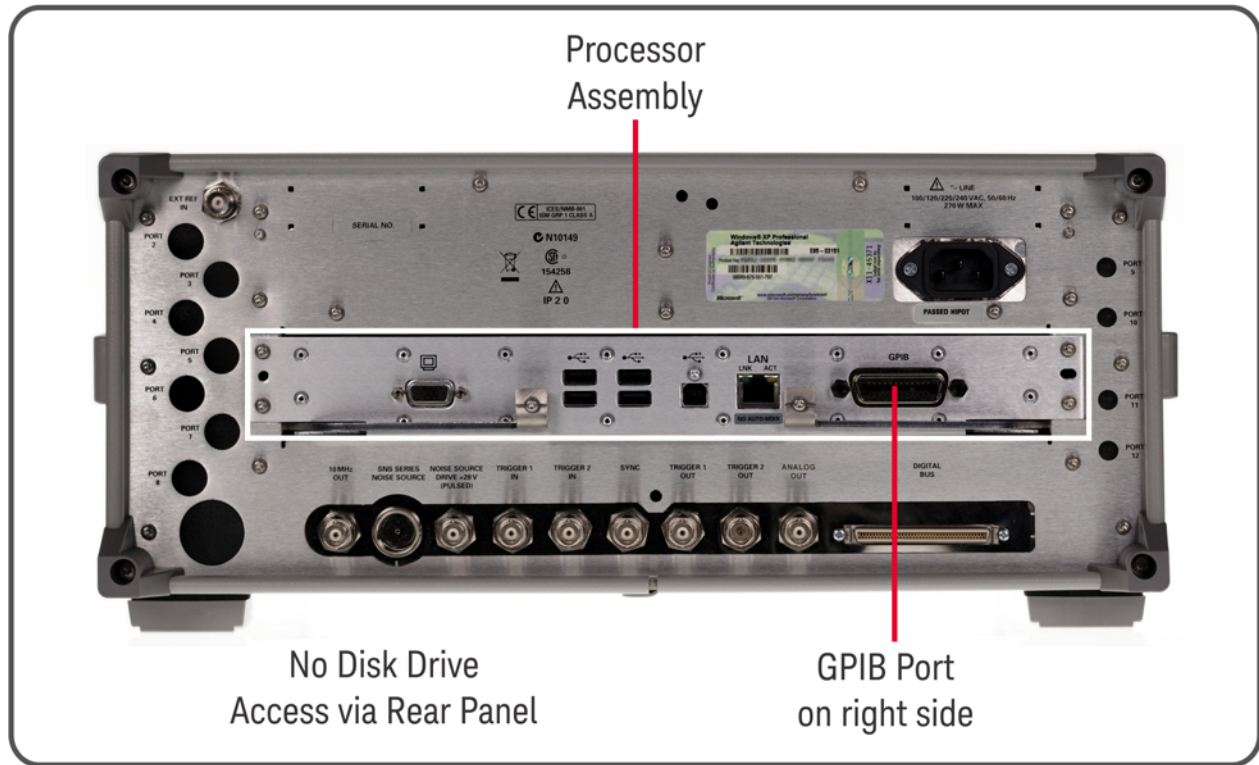


Figure 2-2 Rear Panel of Instrument with Removable Magnetic or Removable Solid-State Disk

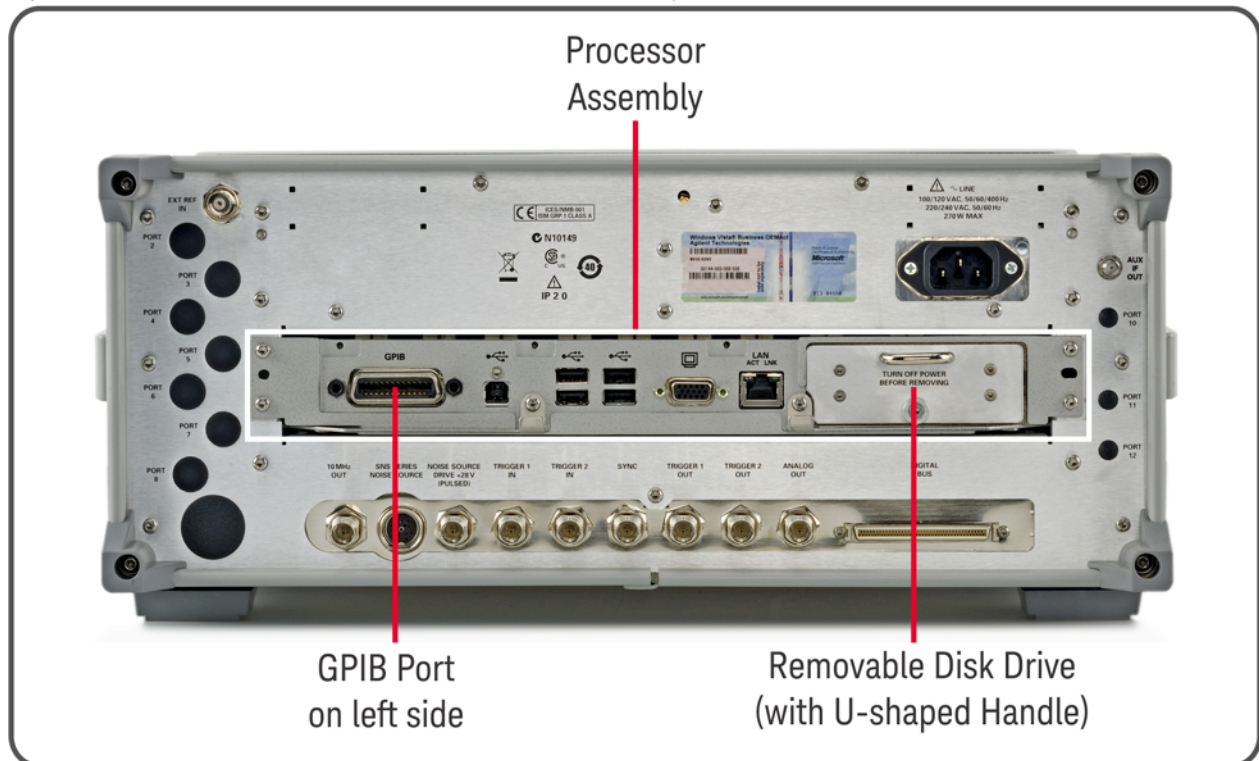

Determining Installed Options

Use the following procedure to determine whether your instrument has a magnetic or solid-state disk drive, and whether Options PC2/PC4 (Dual-Core Processor), or PC3/PC5 (Single-Core Processor) are installed.

1. Using the instrument front panel and softkey menus, press **System** > **Show** > **System**.
2. The "Show System" display appears. Look for start of the "Option" listing, a few lines below the top of the table, as shown in [Figure 2-3](#) below.

Figure 2-3 Show System Display: Option Listing

Installed
Options
List



Agilent Technologies	
MXA	Signal Analyzer
Product Number	N9020A
Serial Number	US01020035
Instrument SW Revision	A.04.00_R0011
Computer Name	A-N9020A-20035
IP Address	127.0.0.1
Host ID	N9020A,US01020035
mDNS Enabled	Yes
mDNS Host Name	A-N9020A-20035
mDNS Service Name	Agilent N9020A Signal Analyzer -
Option	Name / Description
N9020A-IDE	FUJITSU MHT2030AT

3. If the Option list includes "N90X0A-SSD" (where "X" is a digit between 0 and 3, according to the Model Number), then a **Removable Solid-State** disk drive is installed (either because the instrument was supplied with this drive, or because Option SSD has been installed).

If your instrument has a **Fixed Magnetic** or **Removable Magnetic** disk drive, then "N90X0A-IDE" is listed, as shown in [Figure 2-3](#) above.

4. If the Option list includes "N90X0A-PC2" (where "X" is a digit between 1 and 3, according to the Model Number), then Option PC2 is installed.
5. If the Option list includes "N90X0A-PC3" (where "X" is a digit between 0 and 1, according to the Model Number), then Option PC3 is installed.
6. If the Option list includes "N90X0A-PC4" (where "X" is a digit between 1 and 3, according to the Model Number), then Option PC4 is installed.
7. If the Option list includes "N90X0A-PC5" (where "X" is a digit between 0 and 1, according to the Model Number), then Option PC5 is installed.

To dismiss the "Show System" display, press any other front-panel or menu key.

Products Covered by this Document
Determining Instrument Configuration based on Product Name

3 Security Terms and Definitions

Term	Definition
Clearing	As defined in Section 8-301a of DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”, clearing is the process of eradicating the data on media before reusing the media in an environment that provides an acceptable level of protection for the data that was on the media before clearing. Hence, clearing is typically used when the instrument is to remain in an environment with an acceptable level of protection.
Instrument Declassification	A term that refers to procedures that must be undertaken before an instrument can be removed from a secure environment, such as is the case when the instrument is returned for calibration. Declassification procedures include memory sanitization or memory removal, or both. Keysight declassification procedures are designed to meet the requirements specified in DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”, Chapter 8.
Sanitization	<p>As defined in Section 8-301b of DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”, sanitization is the process of removing the data from media before reusing the media in an environment that does not provide an acceptable level of protection for the data that was in the media before sanitizing. Hence, instrument sanitization is typically required when an instrument is moved from a secure to a non-secure environment, such as when it is returned to the factory for calibration.</p> <p>Keysight memory sanitization procedures are designed for customers who need to meet the requirements specified by the US Defense Security Service (DSS). These requirements are specified in the “Clearing and Sanitization Matrix” in Section 5.2.5.5.5 of the ISFO Process Manual for the Certification and Accreditation of Classified Systems under the NISPOM.</p>
Secure Erase	Secure Erase is a term that is used to refer to either the clearing or sanitization features of Keysight instruments.

4 Instrument Memory & Volatility

This chapter summarizes all memory types in the instrument, for the following processor assembly and disk drive configurations:

- a. [Single-Core, Fixed Disk](#) processor assemblies,
- b. [Single-Core, Removable Disk](#) and [Dual-Core, Removable Disk](#) processor assemblies.

For definition of terms, and to determine the configuration of your instrument, based on its Product Name and installed options, see [“X-Series Processor and Disk Drive Configurations” on page 10](#).

The descriptions below are divided between:

1. [Non-Volatile Memory](#),
2. [Volatile Memory](#).

Instrument Memory & Volatility

Non-Volatile Memory

Non-Volatile Memory

This section contains information on the memory components available in your instrument.

- [Table 4-1 on page 20](#) describes memory components that are present in all instruments.
- [Table 4-2 on page 24](#) describes additional memory components that are present only in PXA and some MXA instruments.

Both tables provide details of the size of each memory component, its type, how it is used, its location, volatility, and the sanitization procedure.

NOTE The instrument contains no user-accessible non-volatile memory, except for the Disk Drive described in Item 1 of [Table 4-1](#). For this reason, as indicated in the tables below, no sanitization procedure is required for any memory component except the Disk Drive.

Table 4-1 Summary of Non-Volatile instrument memory - All Instruments (Single-Core and Dual-Core Processors)

Memory Component, Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks	Sanitization Procedure
1. Disk Drive Fixed Magnetic: 40 GByte Removable Magnetic: 160 GByte Removable Solid-State Original: 32 GByte New: 80 GByte This drive is partitioned, as detailed in "Disk Drive Partitioning" on page 26 .	Yes	Yes	Contains operating system, Instrument Software, Factory Calibration Data, Diagnostic software, Crash recovery image, user instrument states, user data files, user trace data and any user installed third party software.	Programmed before installation or by factory/service center calibration procedure software, or by upgrade installation software. Also programmed via operations and by the user.	Single-Core, Fixed Disk: A4 Processor Assy. Single-Core, Removable Disk and Dual-Core, Removable Disk: Rear Panel (Removable) Contains user data.	See Table 5-1 on page 29 .
2. CPU BIOS (CMOS NVRAM) 256 Byte (battery backed)	No	Yes	Contains default BIOS settings to use when booting the Processor Assembly.	Programmed by factory. Settings can be toggled by user.	A4 Processor Assy. Battery backed to maintain Windows calendar time. Contains no user data.	None.
3. License Storage Memory (EEPROM) 512 kbit	No	Yes	Contains instrument serial number and license keys for measurement applications. License keys are encrypted.	Programmed before installation and by installing new license keys.	A7 Midplane Assy. Contains no user data.	None.

Table 4-1 Summary of Non-Volatile instrument memory - All Instruments (Single-Core and Dual-Core Processors)

Memory Component, Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks	Sanitization Procedure
4. Config & Cal Memory (EEPROM) 8 kbit (1024 x 8)	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A14 Synthesizer Assy. Contains no user data.	None.
5. Config Memory (EEPROM) 8 kbit (1024 x 8)	No	Yes	Contains measurement and control software, which is preloaded into FPGA during instrument power-up.	Programmed before installation.	A14 Synthesizer Assy. Contains no user data.	None.
6. Config & Cal Memory (EEPROM) 8 kbit (1024 x 8)	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A15 Front End Control Assy. Contains no user data.	None.
7. Config Memory (Flash) 2 Mbit	No	Yes	Contains measurement and control software, which is preloaded into FPGA during instrument power-up. Primarily YTF, attenuator, and front end switch control.	Programmed before installation.	A15 Front End Control Assy. Contains no user data.	None.
8. Config & Cal Memory (EEPROM) 8 kbit (1024 x 8)	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A2 Analog IF Assy. Contains no user data.	None.
9. Control Logic Memory (CPLD) 1600 Gates	No	Yes	Contains control algorithms to optimize filter performance.	Programmed before installation.	A2 Analog IF Assy. Contains no user data.	None.
10. Config & Cal Memory (EEPROM) 8 kbit (1024 x 8)	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A3 Digital IF Assy. Contains no user data.	None.

Instrument Memory & Volatility

Non-Volatile Memory

Table 4-1 Summary of Non-Volatile instrument memory - All Instruments (Single-Core and Dual-Core Processors)

Memory Component, Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks	Sanitization Procedure
11. Config Memory (Flash) 8 Mbit	No	Yes	Contains measurement and control software, which is preloaded into FPGA during instrument power-up.	Programmed before installation.	A3 Digital IF Assy. Contains no user data.	None.
12. Control Logic Memory (CPLD) 6400 Gates	No	Yes	Contains measurement and control algorithms to optimize digital filtering.	Programmed before installation.	A3 Digital IF Assy. Contains no user data.	None.
13. Serial Presence Detect Memory (EEPROM) 2 Mbit	No	Yes	Used on commercial SDRAM Module, programmed by chip vendor. Contains module identification information.	Programmed by IC vendor only.	A3 Digital IF Assy. Contains no user data.	None.
14. Config & Cal Memory (EEPROM) 8 kbit (1024 x 8)	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A16 Reference Assy. Contains no user data.	None.
15. FPGA Config Memory (EEPROM) 2 Mbit	No	Yes	Contains measurement and control software.	Programmed before installation.	A16 Reference Assy. Contains no user data.	None.
16. Digital Potentiometer (EEPROM) 112 bits (14 Bytes)	No	Yes	Contains default data to preset digital potentiometers during power-up.	Programmed before installation.	A16 Reference Assy. Contains no user data.	None.
17. Front Panel EEPROM 64 kbit	No	Yes	Contains software for running front panel microcontroller. Operates front panel LEDs, and transmits key presses to processor.	Programmed before installation.	A1A2 Front Panel Interface Board Contains no user data.	None.
18. Front Panel CPLD 800 Gates	No	Yes	Contains fixed digital logic associated with front panel keyboard button operation and LEDs.	Programmed before installation at the factory only.	A1A2 Front Panel Interface Board Contains no user data.	None.

Table 4-1 Summary of Non-Volatile instrument memory - All Instruments (Single-Core and Dual-Core Processors)

Memory Component, Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks	Sanitization Procedure
19. EDID Memory (EEPROM) 2 kbit	No	Yes	Extended Display Identification Data is a VESA standard data format that contains basic information about a monitor and its capabilities, including vendor information, maximum image size, color characteristics, factory pre-set timings, frequency range limits, and character strings for the monitor name and serial number.	Programmed before installation.	A1A2 Front Panel Interface Board. Contains no user data.	None.
20. A11 Config Memory (EEPROM) 8 kbit	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A11 Low Band Switch. Contains no user data.	None.
21. A12 Config Memory (EEPROM) 8 kbit	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A12 YTF Assembly. Contains no user data.	None.
22. A13 Config Memory (EEPROM) 8 kbit	No	Yes	Header EEPROM used to identify the assembly.	Programmed before installation.	A13 Front End Assembly. Contains no user data.	None.
23. A18 Header Memory. (EEPROM) 8 kbit	No	Yes	Contains header information used to identify the assembly.	Programmed before installation.	A18 BBIQ Connector Assembly. Contains no user data.	None.
24. A19 Header Memory. (EEPROM) 8 kbit	No	Yes	Contains header information used to identify the assembly.	Programmed before installation.	A19 BBIQ Main Assembly. Contains no user data.	None.
25. Config Memory (Flash) 2 Mbit	No	Yes	Contains measurement and control software, which is preloaded into FPGA during instrument power-up.	Programmed before installation.	A19 BBIQ Main Assembly. Contains no user data.	None.
26. Config Memory (Flash) 32 Mbit	No	Yes	Contains measurement and control software, which is preloaded into FPGA during instrument power-up.	Programmed before installation.	A19 BBIQ Main Assembly. Contains no user data.	None.

Instrument Memory & Volatility

Non-Volatile Memory

The memory components listed in [Table 4-2](#) below are present in:

- all PXA instruments,
- all MXA instruments with serial numbers higher than or equal to MY/SG/US5233,
- MXA instruments with serial numbers lower than MY/SG/US5233, but with Options B85, B1A or B1X.

Table 4-2 Summary of Non-Volatile instrument memory - Additional Components for all PXA Instruments and some MXA Instruments

Memory Component, Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks	Sanitization Procedure
1. Boot ROM (Flash) 8 MByte	No	Yes	Contains the boot ROM, operating system and run-time code for the WBDIF CPU.	Programmed by factory at installation time, or during firmware upgrade.	A26 WBDIF assembly ^a Contains no user data.	None.
2. (Flash) 16 MByte (2 x 64 Mbit)	No	Yes	Contains up to 3 WBDIF FPGA images.	Programmed by factory at installation time, or during FPGA upgrade process.	A26 WBDIF assembly ^a Contains no user data.	None.
3. (EEPROM) 512 Byte	No	Yes	Contains header information used to identify the assembly, and configuration information used to initialize the PCI bus.	Programmed before installation.	A26 WBDIF assembly ^a Contains no user data.	None.
4. (EEPROM) 1024 byte	No	Yes	Contains configuration information used during initialization of the PCI bus. This component is currently unprogrammed.	Programmed before installation.	A26 WBDIF assembly ^a Contains no user data.	None.
5. (CPLD) 256 Macrocells	No	Yes	Contains critical hardware control algorithms.	Programmed before installation.	A26 WBDIF assembly ^a Contains no user data.	None.
6. A16A1 Header Memory (EEPROM) 8 kbit	No	Yes	Contains header information used to identify the assembly.	Programmed before installation.	A16A1 Reference Daughter Assembly ^b Contains no user data.	None.
7. Config Memory (Flash) 1 Mbit	No	Yes	Contains measurement and control software, which is preloaded into FPGA during instrument power-up.	Programmed before installation.	A16A1 Reference Daughter Assembly ^b Contains no user data.	None.

Table 4-2 Summary of Non-Volatile instrument memory - Additional Components for all PXA Instruments and some MXA Instruments

Memory Component, Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks	Sanitization Procedure
8. A25 Header Memory (EEPROM) 8 kbit	No	Yes	Contains header information used to identify the assembly.	Programmed before installation.	A25 WBAIF ^a Contains no user data.	None.
9. Control Logic Memory (CPLD) 1600 Gates	No	Yes	Contains control algorithms.	Programmed before installation.	A25 WBAIF ^a Contains no user data.	None.
10. Config Memory (Flash) 2 Mbit	No	Yes	Contains measurement and control software, which is preloaded into FPGA during instrument power-up.	Programmed before installation.	A25 WBAIF ^a Contains no user data.	None.

- a. Present in all PXA instruments, and MXA instruments with Options B85, B1A or B1X.
- b. Present in all PXA instruments, all MXA instruments with serial numbers higher than or equal to MY/SG/US5233, and MXA instruments with serial numbers lower than MY/SG/US5233, but with Options B85, B1A or B1X.

Instrument Memory & Volatility

Non-Volatile Memory

Disk Drive Partitioning

The instrument's disk drive is divided at the factory into three visible partitions, labeled C:, D: and E:, plus a fourth hidden partition.

The sizes of each partition vary according to the instrument's [Disk Drive Configuration](#).

Details of the sizes and functions of all partitions are provided in [Table 4-3](#) below.

Table 4-3 Disk Drive Partitions

Partition Label	Size (GBytes)	Purpose
C:	Fixed Magnetic: 15 GB Removable Magnetic: 62 GB Removable Solid-State: (Original) 16 GB (New) 32 GB	Primary partition for applications and secondary data.
D:	Fixed Magnetic: 6 GB Removable Magnetic: 23 GB Removable Solid-State: (Original) 3.75 GB (New) 17 GB	Default location for user data.
E:	Fixed Magnetic: 6 GB Removable Magnetic: 2.3 GB Removable Solid-State: (Original) 1.6 GB (New) 2 GB	Calibration data.
Hidden	Fixed Magnetic: 6.5 GB Removable Magnetic: 54 GB Removable Solid-State: (Original) 8.2 GB (New) 23 GB	Factory recovery image of the C: partition.

Volatile Memory

The volatile memory in the instrument does not have battery backup. It does not retain any information when AC power is removed.

Removing power from this memory meets the memory sanitization requirements specified in the “Clearing and Sanitization Matrix” in Section 5.2.5.5.5 of the [ISFO Process Manual for the Certification and Accreditation of Classified Systems under the NISPOM](#).

Table 4-4 Summary of Volatile Instrument Memory - Instruments with Single-Core and Dual-Core Processors

Memory Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks	Sanitization Procedure
1. Processor SDRAM Single-Core, Fixed Disk: 1 GByte or 2 GByte Single-Core, Removable Disk: 4 GByte Dual-Core, Removable Disk: 4 GByte or 8 GByte	Yes	No	Main dynamic RAM memory for processor. Contains working copies of operating system, instrument measurement applications, calibration data, and measurement data.	Programmed before installation, or by factory/service center calibration procedure software, or by firmware upgrade installation software. Also programmed via firmware operations and by user.	A4 Processor Assy. Contains user data.	Turn off instrument power. ^a
2. SDRAM 256 MByte	Yes	No	Contains measurement data from data acquisition system.	Programmed by firmware. Not accessible by user.	A3 Digital IF Assy. Contains raw measurement data.	Turn off instrument power. ^a
3. SDRAM 2 GByte	Yes	No	Contains measurement data from data acquisition system.	Programmed by firmware. Not accessible by user.	A3 Digital IF Assy. For all N9030A instruments, and instruments with Options DP2, B40, MPB Contains raw measurement data.	Turn off instrument power. ^a
4. SDRAM 2 GByte Module + 256 MByte Module	Yes	No	Contains measurement data from data acquisition system.	Programmed by firmware. Not accessible by user.	A26 Wideband Digital IF Assy. Contains raw measurement data.	Turn off instrument power. ^a

a. This memory is **not** battery backed-up or connected to standby power.

Instrument Memory & Volatility
Volatile Memory

5 Memory Clearing, Sanitization and Removal Procedures

This section explains how to clear, sanitize, and remove memory from your instrument, for all types of non-volatile memory that can be written to during normal instrument operation.

Table 5-1 Disk Drive

Description and purpose	The Disk Drive is the main memory for the instrument. It has very large storage capacity, plus fast read and write times. There are no limitations on the number of read/write cycles. It contains the operating system, Instrument Software, Factory Calibration Data, Diagnostic software, Crash recovery image, user instrument states, user data files, user trace data and any user-installed third party software. The Disk Drive is written to frequently by the operating system and other application software.
Size	Fixed Magnetic magnetic disk drive: 40 Gigabytes Removable Magnetic disk drive: 160 Gigabytes Removable Solid-State disk drive: 32 Gigabytes (original) or 80 Gigabytes (new)
Memory clearing	Software utilities are available that comply with the clearing requirements specified for Magnetic Disks and Flash Drives in the "Clearing and Sanitization Matrix" in Section 5.2.5.5.5 of the ISFO Process Manual for the Certification and Accreditation of Classified Systems under the NISPOM .
Memory sanitization	We recommend always removing the Disk Drive to achieve sanitization. For program classifications lower than Top Secret, the disk can be sanitized using method "d" (for magnetic disks) or method "c" followed by "h" (for solid-state drives) as defined in the "Clearing and Sanitization Matrix" in Section 5.2.5.5.5 of the ISFO Process Manual for the Certification and Accreditation of Classified Systems under the NISPOM . For Top Secret and higher program classifications, Disk Drive removal is the only acceptable sanitization procedure.
Memory removal	Single-Core, Fixed Disk Processor assembly: see "Instruments with Non-Removable Drives" on page 44, in the Chapter "Disk Drive Removal Procedure". Single-Core, Removable Disk or Dual-Core, Removable Disk Processor assemblies: see "Instruments with Removable Drives" on page 45, in the Chapter "Disk Drive Removal Procedure".
Write protecting	The Disk Drive cannot be write protected. The operating system and software must be able to read from and write to the drive during normal operation.
Memory validation	The Disk Drive memory can be validated using third-party Windows utilities.

Table 5-2 CPLD, CMOS Programmable Logic Devices

Description and purpose	These memory devices are used to execute timing, control, and measurement functions. No user data is contained in these devices. This memory cannot be written to during instrument operation.
Size	1600 to 6400 logic gates.

Memory Clearing, Sanitization and Removal Procedures

Table 5-2 CPLD, CMOS Programmable Logic Devices

Memory clearing	Not applicable. This memory does not contain user information and is not accessible by the user.
Memory sanitization	Not applicable. This memory does not contain user information and is not accessible by the user.
Memory removal	Not applicable.
Write protecting	Not applicable.
Memory validation	Not applicable.
Remarks	These devices are programmed in the factory via diagnostic connectors on the PCB assemblies. After instrument assembly, the diagnostic connectors are not physically accessible and not electrically connected.

Table 5-3 EEPROM Memories

Description and purpose	These memories are used to identify the assemblies (header info) and store option configuration data. Some are also used to hold factory software for FPGAs. The software is loaded when the instrument powers up. This memory cannot be written to during instrument operation.
Size	2 kbit to 8 Mbit
Memory clearing	Not applicable. This memory does not contain user information and is not accessible by the user.
Memory sanitization	Not applicable. This memory does not contain user information and is not accessible by the user.
Memory removal	Not applicable.
Write protecting	Not applicable.
Memory validation	Not applicable.
Remarks	<p>With one exception, as described below, these memories are only writable by factory/service center software, or upgrade installation software. These memories are internally connected to proprietary internal control data busses (as opposed to standard computer busses such as IDE, PCI, USB). They are not accessible by the operating system or by third-party software, or by the user, to protect the measurement accuracy and consistency of the instrument. They are rarely modified, to ensure no degradation of instrument performance. These memories contain no user data. Many of these memories have long write times, and limited write endurance, so they are not intended to be written to dynamically by software.</p> <p>The sole exception applies to the EEPROM on the A7 Midplane Assembly. Inserting a USB memory device containing a valid license key file into the instrument causes the key file to be copied to both the C: drive and the EEPROM on the A7 Midplane Assembly.</p>

Instrument Sanitization Procedures

This section includes flowcharts that describe how to sanitize an instrument by physical removal and replacement of either the Processor Assembly or Disk Drive.

- For [Single-Core, Fixed Disk](#) instruments, see [“Replacement of Processor Assembly” on page 31](#).
- For [Single-Core, Removable Disk](#) and [Dual-Core, Removable Disk](#) instruments, see [“Replacement of Disk Drive” on page 33](#).

Application License Key Storage

Note that License keys for most Applications are stored in EEPROM on the A7 Midplane Assembly (as described in Item 3 of [Table 4-1 on page 20](#)). Therefore, when replacing either the Processor Assembly or Disk Drive, you do **not** need to back up and restore the license keys.

The sole exception is the 89601A VSA Application, which uses a Site Key license. For information on how to regenerate a Site Key, see [Regenerating a Site Key License for 89601A VSA Application](#) below.

Regenerating a Site Key License for 89601A VSA Application

When a repair requires the replacement of a Processor Assembly or Disk Drive for an instrument that includes the 89601A VSA Application, you must request a new Site Key License, as if installing 89601A VSA for the first time. Details of how to do this are provided in the following article, available on the Keysight web site:

[How do I recover my VSA 89600S license after a hard drive crash?](#)

NOTE This requirement applies only to the 89601A VSA Application. It does **not** apply to the newer 89601B.

Replacement of Processor Assembly

This procedure applies only to [Single-Core, Fixed Disk](#) instruments.

Refer to the flowchart in [Figure 5-1](#) below for details of how to perform this procedure.

Note that this flowchart differs from that for replacement of the Disk Drive only in that the entire Processor Assembly is replaced. The steps that differ between the two procedures are marked in yellow in the flowcharts.


For details of how to archive or restore the instrument's calibration files (Steps 2, 11 and 15 in the flowchart), see [“Archiving and Restoring Factory Calibration Data Files” on page 35](#).

For details of how to remove the Processor Assembly (Step 5), see [“Processor Assembly Removal Procedure” on page 41](#).

Memory Clearing, Sanitization and Removal Procedures

Instrument Sanitization Procedures

Figure 5-1

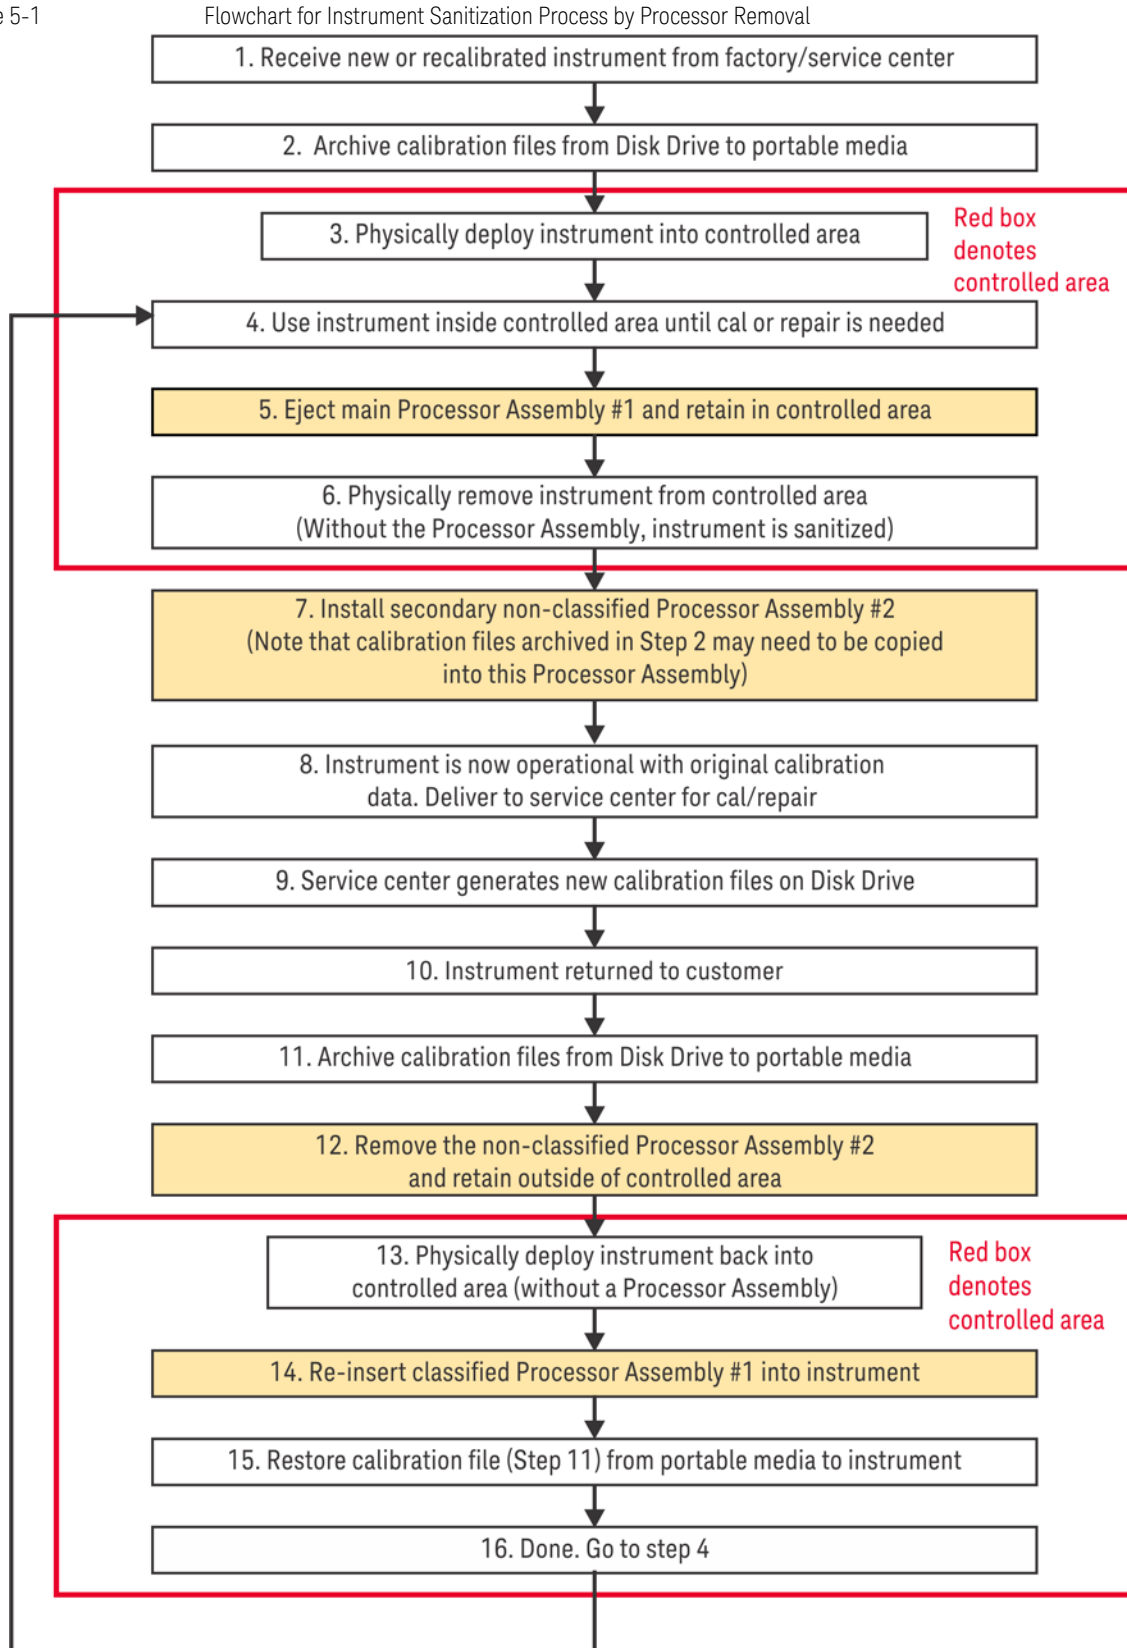

Replacement of Disk Drive

This procedure applies to [Single-Core, Removable Disk](#) and [Dual-Core, Removable Disk](#) instruments.

Refer to the flowchart in [Figure 5-2](#) below for details of how to perform this procedure.

Note that this flowchart differs from that for replacement of the Processor Assembly only in that the removable Disk Drive is replaced. The steps that differ between the two procedures are marked in yellow in the flowcharts.

For details of how to archive or restore the instrument's calibration files (Steps 2, 11 and 15 in the flowchart), see [“Archiving and Restoring Factory Calibration Data Files” on page 35](#).

For details of how to remove the Disk Drive (Step 5), see [“Disk Drive Removal Procedure” on page 43](#).

IMPORTANT


Ensure that the instrument software revision on the secondary non-classified disk drive matches that of the classified drive in the controlled area.

If the non-classified drive receives a software upgrade, or if the non-classified drive is replaced with a drive that contains a newer revision of software than that of the classified drive, the classified drive will require a software upgrade (inside the controlled area) to match the non-classified drive.

Memory Clearing, Sanitization and Removal Procedures

Instrument Sanitization Procedures

Figure 5-2

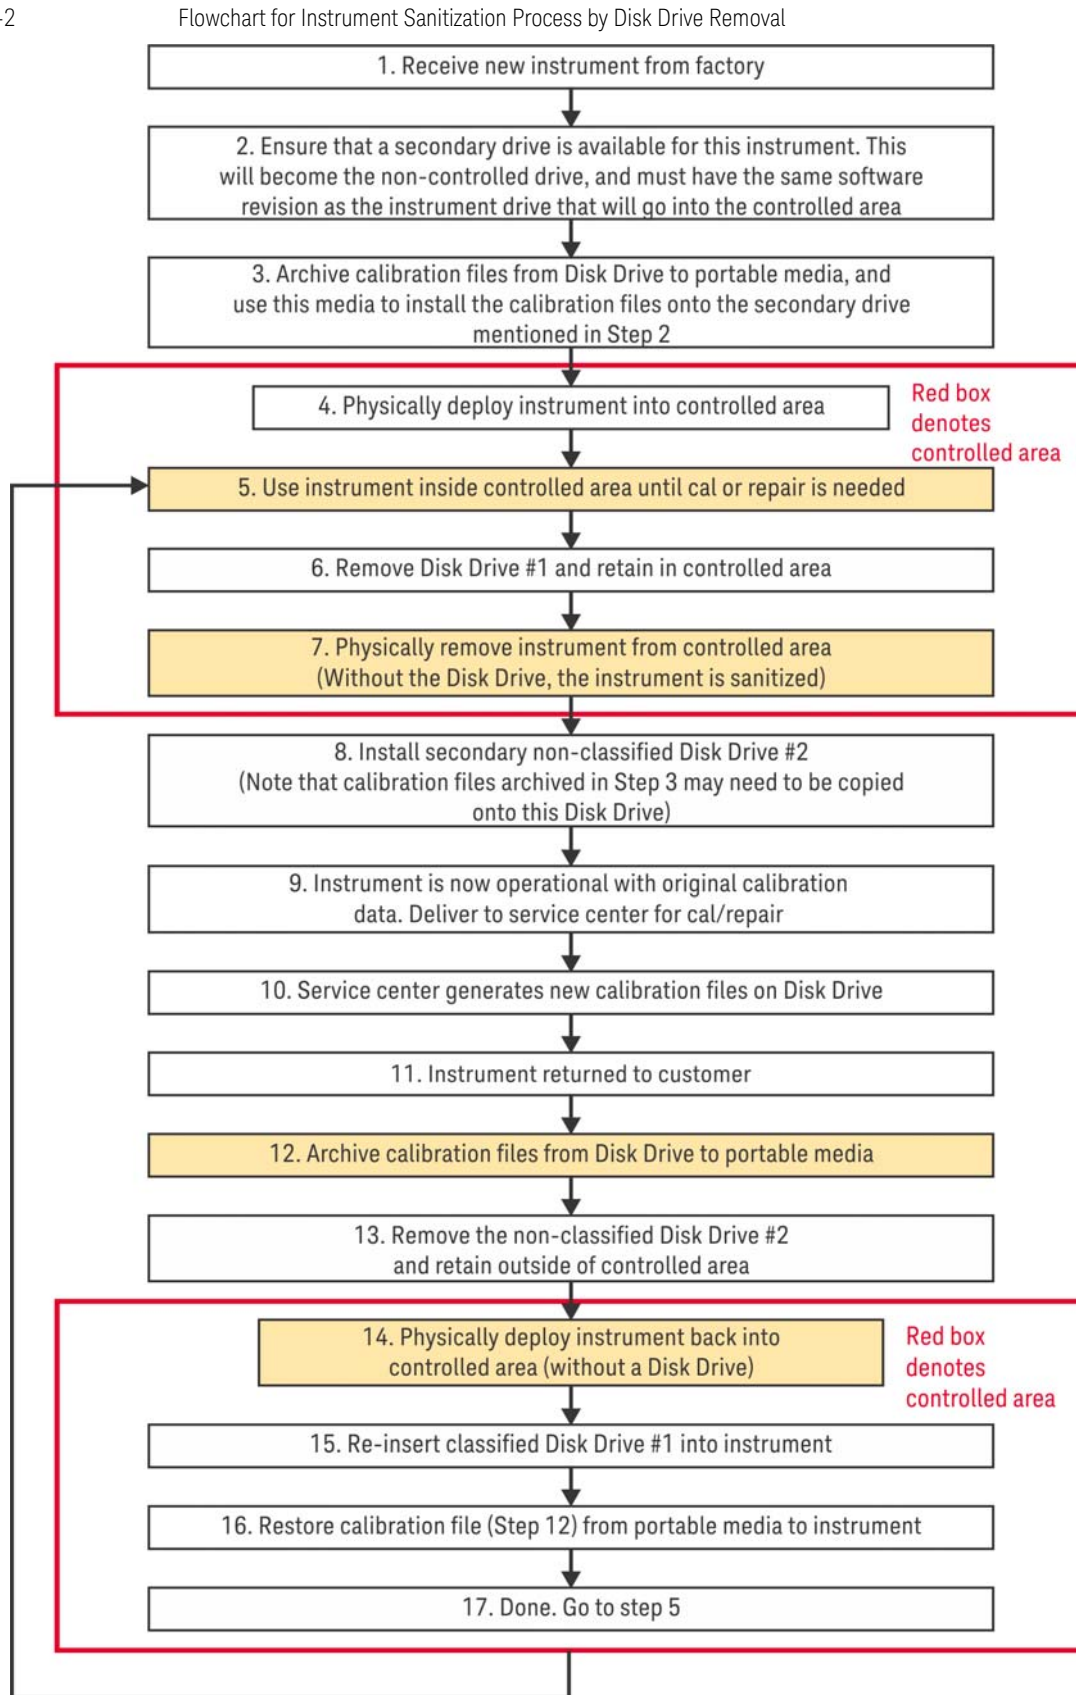

Archiving and Restoring Factory Calibration Data Files

This section describes how to archive ("back up") the instrument's factory calibration data to an external USB memory device, or restore the calibration data from an external memory device.

The backup and restore procedures differ according to the instrument software revision. This section describes the three possible pairs of procedures.

To determine the instrument software revision, follow the procedure ["Determining Instrument Software Revision" on page 36](#) below.

To determine which backup or restore procedures should be used, according to the instrument software revision, see [Table 5-4 on page 37](#).

Tools Required

To perform backup or restore operations, you need:


- a mouse with a USB interface
- a portable memory device with a USB interface
- an alphanumeric keyboard with a USB interface

Determining Instrument Software Revision

1. On the instrument front panel, press **System** > **Show** > **System**.
2. The "Show System" display appears, as shown in [Figure 5-3](#) below. Look for the Software Revision number specified in the "Instrument S/W Revision" entry.

Figure 5-3 Show System Display

Software Revision Entry →

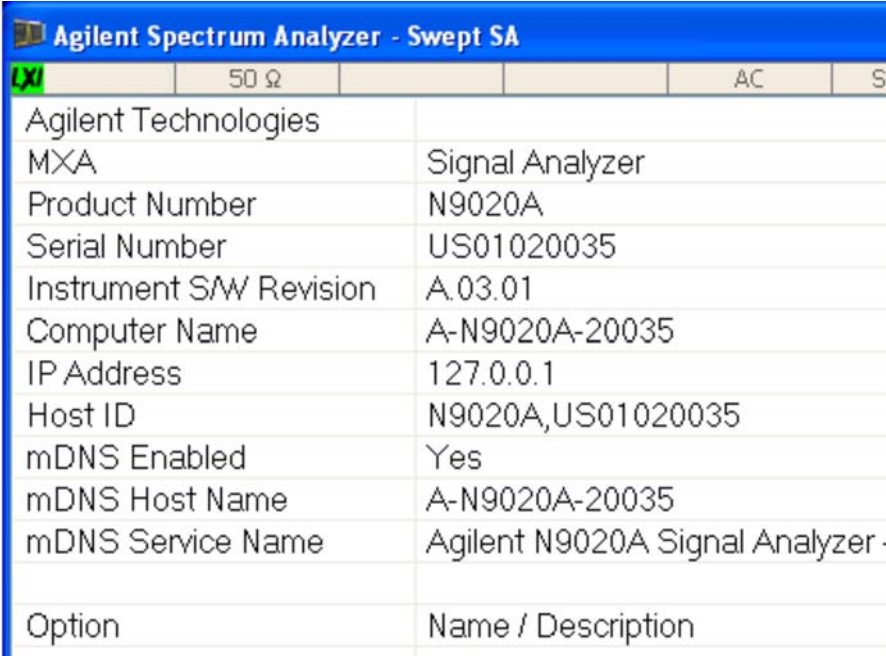

Agilent Spectrum Analyzer - Swept SA	
50 Ω	AC
Agilent Technologies	
MXA	Signal Analyzer
Product Number	N9020A
Serial Number	US01020035
Instrument S/W Revision	A.03.01
Computer Name	A-N9020A-20035
IP Address	127.0.0.1
Host ID	N9020A,US01020035
mDNS Enabled	Yes
mDNS Host Name	A-N9020A-20035
mDNS Service Name	Agilent N9020A Signal Analyzer
Option	Name / Description

3. To dismiss the "Show System" display, press any other front-panel or menu key.

Memory Clearing, Sanitization and Removal Procedures Archiving and Restoring Factory Calibration Data Files

When you have obtained the instrument Software Revision number, refer to [Table 5-4 on page 37](#) below for the appropriate backup or restore procedure.

Table 5-4 Backup & Restore Procedures for all Instrument Software Revisions

Instrument Software Revision	Backup Procedure	Restore Procedure
A.01.55 or lower	See “Data Backup using XML File” on page 37 .	See “Data Restore using XML File” on page 37 .
Greater than A.01.55; lower than A.02.00	See “Data Backup using Utility Program” on page 38 .	See “Data Restore using Utility Program” on page 38 .
A.02.00 or greater	See “Data Backup or Restore using Alignment Data Wizard” on page 39 .	See “Data Backup or Restore using Alignment Data Wizard” on page 39 .

Software Revision A.01.55 or Lower

If the instrument software revision is A.01.55 or lower, the calibration data is stored in an XML database file.

Data Backup using XML File

Follow the steps below:

1. Close the instrument application software by pressing **File > Exit > Enter**.
2. Plug the mouse's USB cable into one of the instrument's USB ports.
3. Plug the USB memory device into another of the instrument's USB ports.
4. Using the mouse, double-click on the Windows Explorer icon on the desktop and navigate to the following folder:
`E:\AlignDataStorage`
5. Copy the following file onto the USB memory device:
`CurrentDataSet.xml`

Data Restore using XML File

The data can be restored from a USB memory device containing the XML database file, by using the following process.

1. Close the instrument application software by pressing **File > Exit > Enter**.
2. Plug the mouse's USB cable into one of the instrument's USB ports.
3. Plug the USB memory device into another of the instrument's USB ports.
4. Using the mouse, double-click on the Windows Explorer icon on the desktop and navigate to a folder on the USB memory device containing a previously-saved calibration data file named:
`CurrentDataSet.xml`
5. Select the calibration data file, then copy it to the Windows clipboard by selecting **Edit > Copy** from the Windows Explorer pull-down menu.
6. Navigate to the folder below and paste the file by selecting **Edit > Paste** from the Windows Explorer pull-down menu:
`E:\AlignDataStorage`
7. Verify that the file `CurrentDataSet.xml` was copied to the new location.
8. Cycle the instrument power.

Software Revision Greater than A.01.55 and Lower than A.02.00

If the instrument software revision is greater than A.01.55, the calibration data is stored in an SQL database file.

Memory Clearing, Sanitization and Removal Procedures Archiving and Restoring Factory Calibration Data Files


For software revisions greater than A.01.55, but lower than A.02.00, the SQL file is written and read by a utility program called `BackupAndRestore.exe`.

Data Backup using Utility Program

Follow the steps below:

1. Close the instrument application software by pressing **File > Exit > Enter**.
2. Plug the mouse's USB cable into one of the instrument's USB ports.
3. Plug the USB memory device into another of the instrument's USB ports.
4. Plug the USB keyboard into another of the instrument's USB ports.
5. Using the mouse double-click on the Windows Explorer icon on the desktop and navigate to the following folder:
`C:\Program Files\Agilent\SignalAnalysis\Physics`
6. Double-click on `BackupAndRestore.exe`. The "Calibration Data Backup And Restore" dialog shown in [Figure 5-4](#) appears.

Figure 5-4 Calibration Data Backup

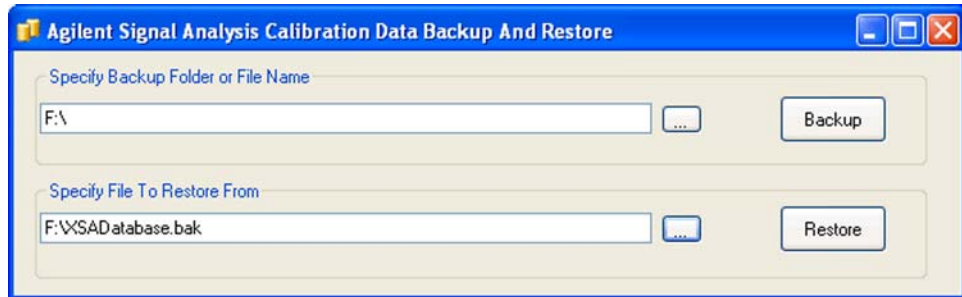


7. In the group box "Specify Backup Folder or File Name" use the mouse to press the "..." button to open the "Browse For Folder" dialog.
8. In the "Browse For Folder" dialog, select or create the desired folder on the USB memory device, then press **OK**.
9. Press **Backup**, then wait for the calibration database to be backed up.
10. When the backup has completed, close the "Calibration Data Backup And Restore" dialog.

Data Restore using Utility Program

Follow the steps below:

1. Close the instrument application software by pressing **File > Exit > Enter**.
2. Plug the mouse's USB cable into one of the instrument's USB ports.
3. Plug the USB memory device into another of the instrument's USB ports.
4. Using the mouse double-click on the Windows Explorer icon on the desktop and navigate to the following folder:
`C:\Program Files\Agilent\SignalAnalysis\Physics`
5. Double-click on `BackupAndRestore.exe`: the "Calibration Data Backup And Restore" dialog shown in [Figure 5-4](#) appears.

Figure 5-5 Calibration Data Backup

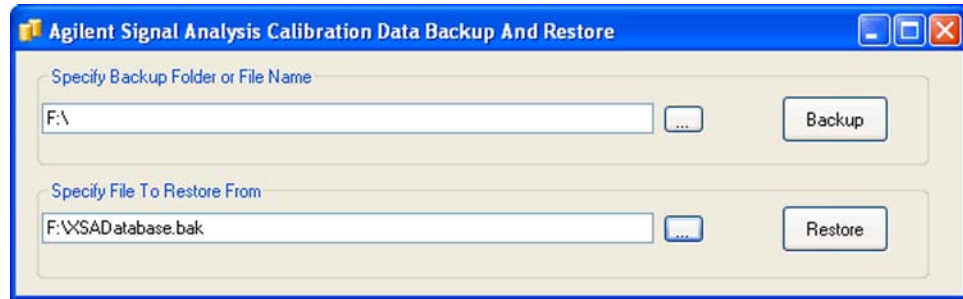

6. In the group box “Specify File To Restore From” use the mouse to press the “...” button to open the “Browse For File” dialog.
7. In the "Browse For File" dialog, select the desired file on the USB memory device, then press **OK**.
8. Press **Restore**, then wait for the calibration database to be restored.
9. When the restore has completed, close the "Calibration Data Backup And Restore" dialog.

Software Revision A.02.00 or Greater

For software revisions A.02.00 or greater, the SQL calibration data file is read and written by the Alignment Data Wizard.

Data Backup or Restore using Alignment Data Wizard


The Alignment Data Wizard is launched directly from the instrument application software interface, so you do **not** need to exit the application software before proceeding.

Follow the steps below to start the wizard:

1. Plug the mouse’s USB cable into one of the instrument’s USB ports.
2. Plug the USB memory device into another of the instrument’s USB ports.
3. Plug the USB keyboard into another of the instrument’s USB ports.
4. Press **System > Alignments > Backup or Restore Align Data...**
5. When prompted, press **OK** to close the instrument application.
6. The Alignment Data Wizard dialog appears, as shown in [Figure 5-6](#) below:

Memory Clearing, Sanitization and Removal Procedures Archiving and Restoring Factory Calibration Data Files

Figure 5-6 Alignment Data Wizard Dialog

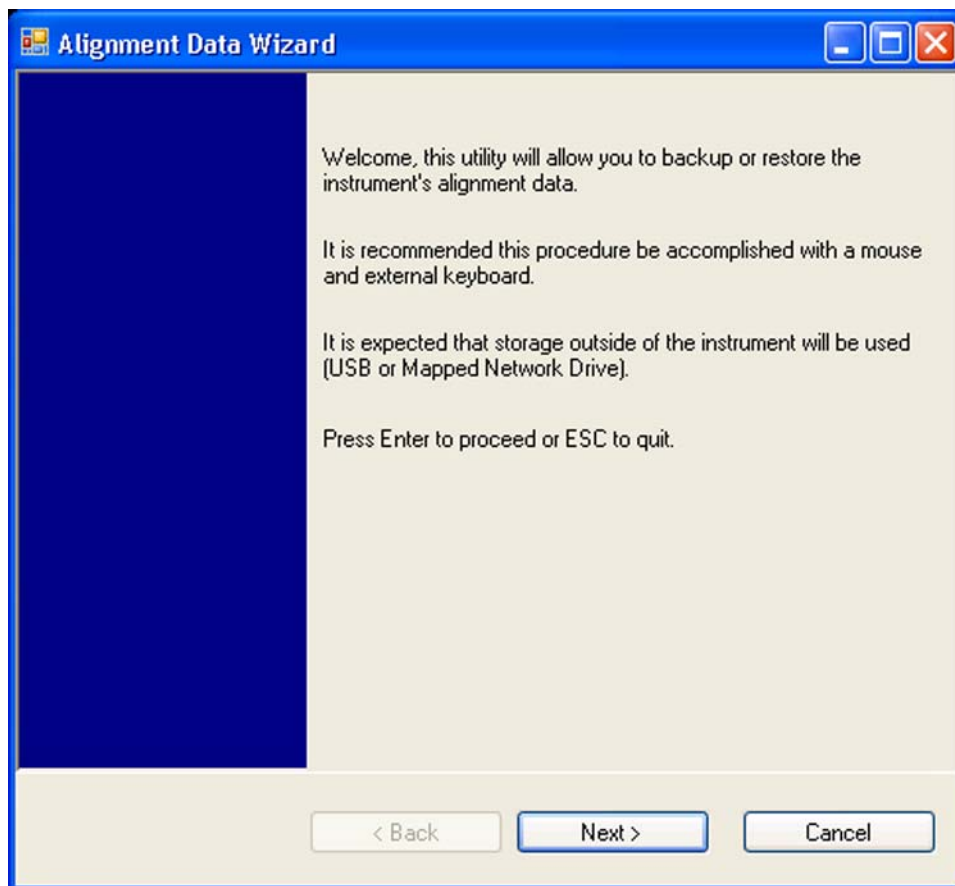

7. Follow the wizard's on-screen instructions to back up the calibration data to the external USB memory device, **or** restore the data from the device.


6 Processor Assembly Removal Procedure

To remove the processor board assembly, follow the procedure below, while referring to [Figure 6-1](#), which shows the rear panel of instruments with [Single-Core, Fixed Disk](#) processor assemblies.

The procedure for instruments with [Single-Core, Removable Disk](#) or [Dual-Core, Removable Disk](#) processor assemblies is identical, although the appearance of the rear panel differs from that shown in [Figure 6-1](#). (For comparative illustrations of the rear panel types, see [“Rear Panel Configurations”](#) on page 14.)

CAUTION Before removing the Processor Assembly, ensure that the instrument’s power is turned off.

Figure 6-1 Processor Assembly Removal Procedure

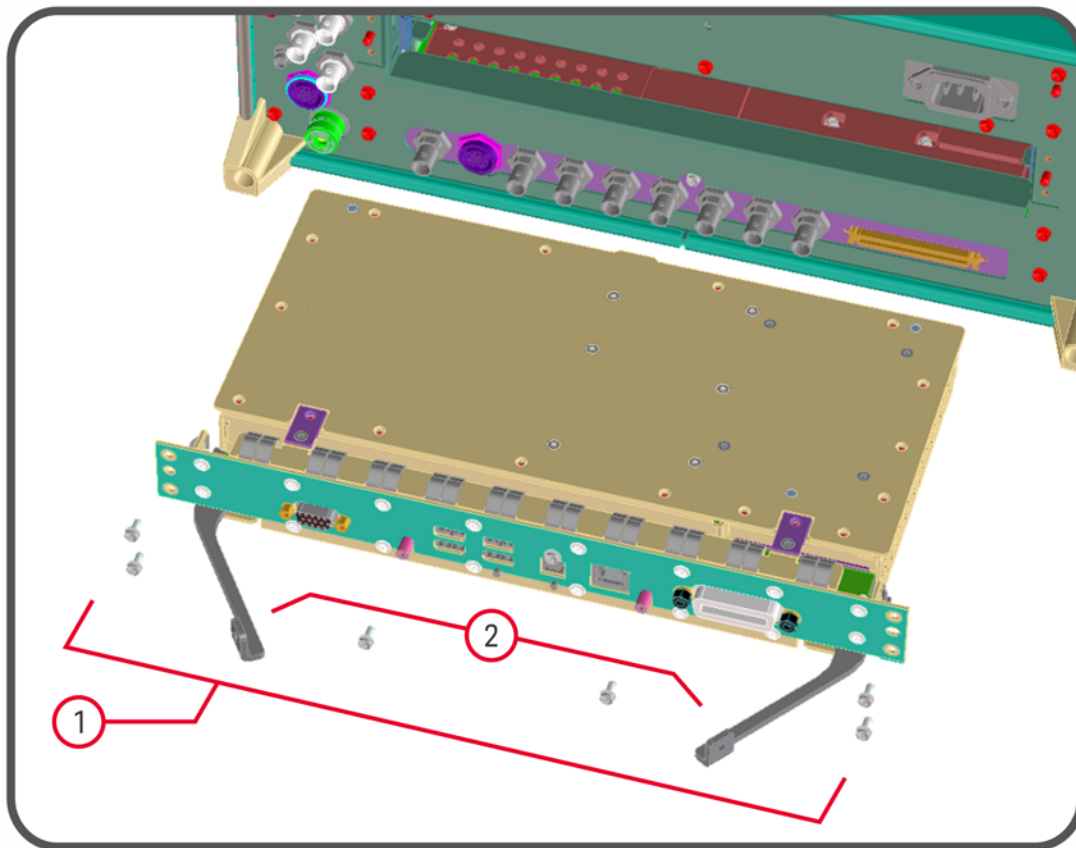

Processor Assembly Removal Procedure

1. Locate and remove the Processor Assembly from the instrument, by removing the 6 rear panel screws (part number 0515-0372, M3 x 0.5, 8 mm long).
2. The assembly can be removed from the chassis by pulling it straight out. Use the two ejector arms to remove the Assembly from the instrument

TIP

Most Application License keys are stored in EEPROM on the A7 Midplane Assembly (as described in Item 3 of [Table 4-1 on page 20](#)). Therefore, when replacing the Processor Assembly, you do **not** need to back up and restore the license keys.

The sole exception is the license key for the 89601A VSA Application. For information about how to regenerate these licenses, see [“Regenerating a Site Key License for 89601A VSA Application” on page 31](#).

7 Disk Drive Removal Procedure

This chapter describes the procedures for physical removal of the disk drive from:

- a. [Instruments with Non-Removable Drives](#) (generally, older MXA, EXA and CXA instruments),
- b. [Instruments with Removable Drives](#) (generally, all PXA instruments, and newer MXA, EXA and CXA instruments).

For detailed information about the drive types installed in each instrument type, see the section [“X-Series Processor and Disk Drive Configurations” on page 10](#), in the Chapter [Products Covered by this Document](#).

TIP

Most Application License keys are stored in EEPROM on the A7 Midplane Assembly (as described in Item 3 of [Table 4-1 on page 20](#)). Therefore, when replacing the Disk Drive, you do **not** need to back up and restore the license keys.

The sole exception is the license key for the 89601A VSA Application. For information about how to regenerate these licenses, see [“Regenerating a Site Key License for 89601A VSA Application” on page 31](#).


When installing a replacement Disk Drive, ensure that the instrument software revision on the replacement drive matches that of the original drive.

Instruments with Non-Removable Drives

To remove the disk drive, follow the procedure below, while referring to [Figure 7-1](#). The numbered items in the figure correspond to the step numbers in the procedure.

Before commencing this procedure, remove the complete Processor Assembly from the instrument, following the procedure described in the chapter [Processor Assembly Removal Procedure](#).

Figure 7-1 Disk Drive Removal Procedure

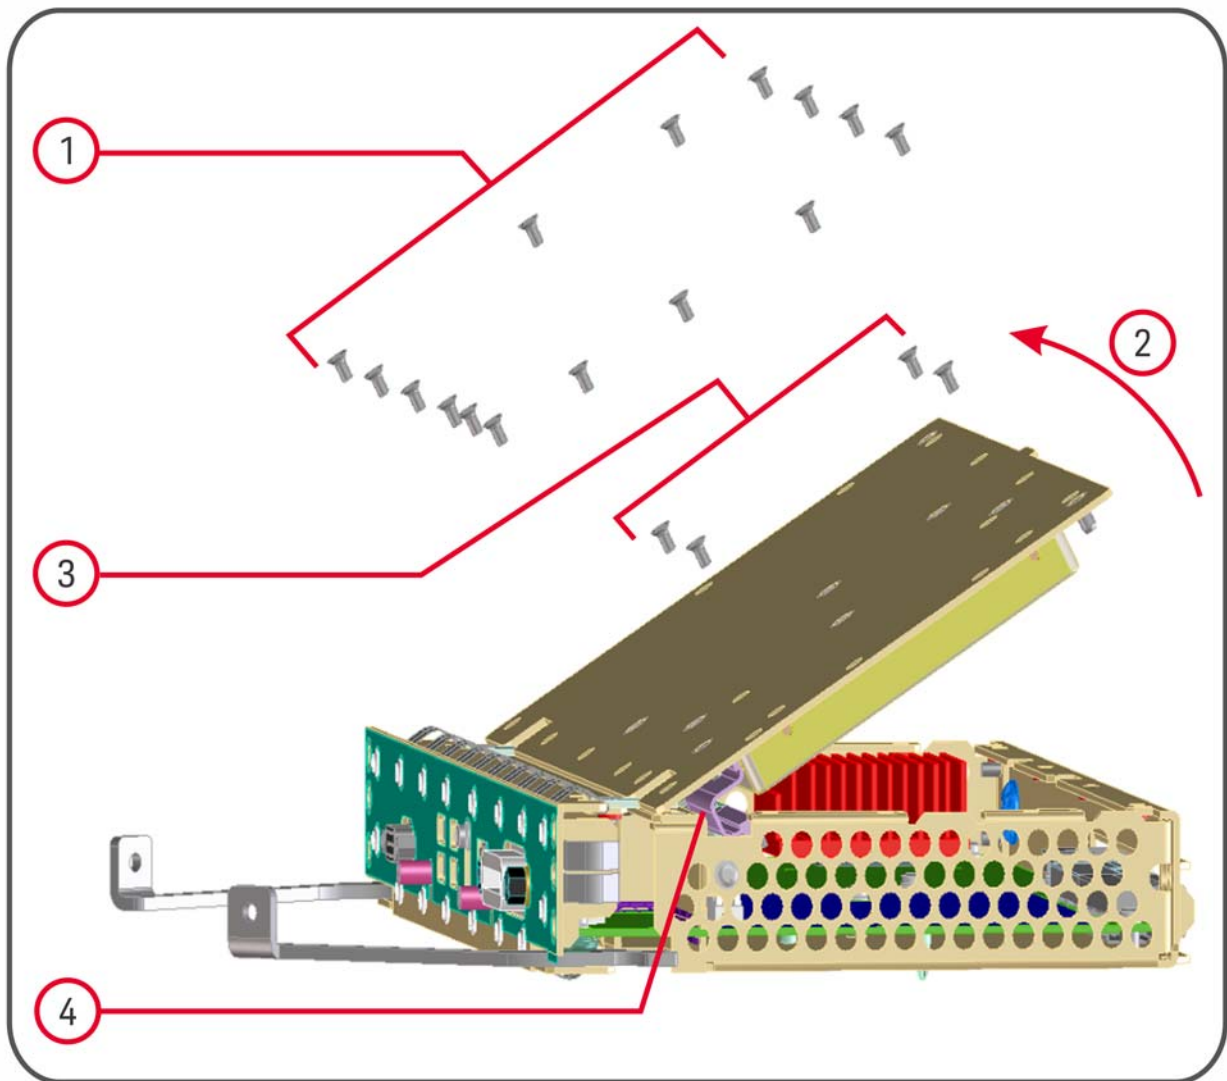

1. Remove 15 screws from the top lid of the Processor Assembly.
2. Tilt the lid up.
3. While holding the disk drive to prevent it from falling, remove the 4 drive retaining screws.
4. Disconnect the drive cable from the disk drive.

Instruments with Removable Drives

To remove the disk drive, follow the procedure below. You do **not** need to remove the Processor Assembly from the instrument before removing the drive.

The numbered items in the figures below correspond to the step numbers in the procedure.

CAUTION Before removing the disk drive, ensure that the instrument's power is turned off.

1. Locate the Processor and Disk Drive Assembly on the instrument's rear panel, as shown in [Figure 2-2](#) in the section "[Rear Panel Configurations](#)" on page 14. In [Figure 7-2](#) below, the processor assembly is shown removed from the rear panel for clarity.


Figure 7-2 Processor Assembly with Removable Disk Drive



2. Locate the removable drive, and its retaining thumbscrew, as shown in [Figure 7-2](#).
3. Turn the thumbscrew to release the drive from the panel, as shown in [Figure 7-3](#) below. If the thumbscrew is too tight to turn by hand, use a TORX T10 screwdriver to loosen it.

Disk Drive Removal Procedure Instruments with Removable Drives

Figure 7-3 Removable Disk Drive Unit partially extracted

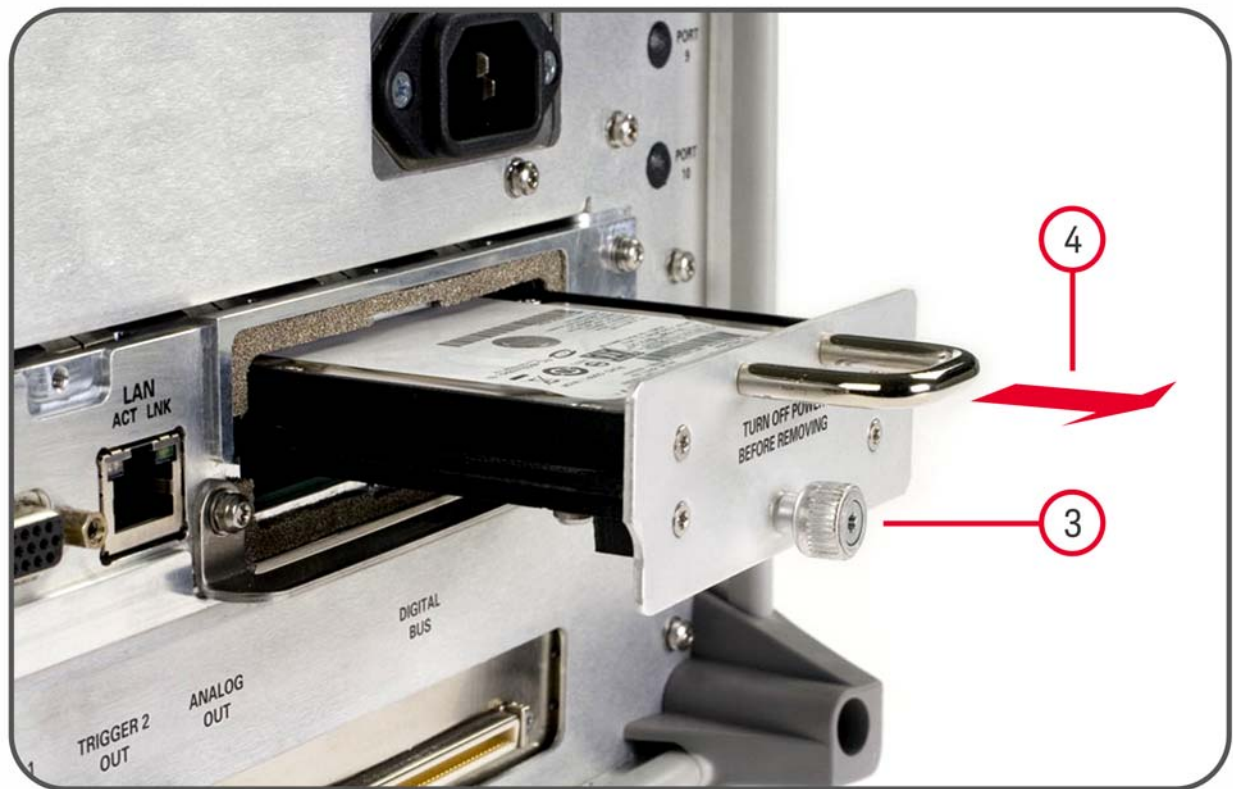

4. Pull the U-shaped handle attached to the drive unit, to remove the drive from the Processor Assembly, as shown in [Figure 7-3](#).

8 User and Remote Interface Security Measures

This chapter discusses options that are available to you to control and configure remote access to the instrument, including:

- [SCPI/GPIB Control of Interfaces](#)
- [Operating System Security Features](#)
- [USB Interfaces](#). This topic includes information about how to set the instrument's USB ports to read-only.

IMPORTANT

Users are responsible for providing security for the I/O ports for remote access, by controlling physical access to the I/O ports. The I/O ports must be controlled because they provide access to most user settings, user states, and the display memory.

SCPI/GPIB Control of Interfaces

The GPIB command `LLLO` (local lockout) can be sent by the controller to disable operation of the instrument's front-panel keys and softkey menus.

However, sending the `LLLO` command does **not** disable access to the instrument via its USB ports. For details of how to restrict the operation of the USB ports, see ["Configuring USB for Read-only"](#) on page 51 below.

Operating System Security Features

The instrument's Windows operating system includes a variety of features that you can invoke or modify to enhance system security. These include the following:

- The ability to create custom user accounts, and assign different security levels to each account by adding it to an existing group. The group types predefined by Windows are: Administrator, Power User, User, Backup Operator, and Guest, but you can also define new group types.
- To provide additional protection for instruments that have a network (or internet) connection, the standard Windows Firewall is enabled by default.
- You can install standard third-party antivirus and spyware detection software designed for use with Windows. If your instrument has a network (or internet) connection, this may be advisable.

CAUTION Running any third-party program while making measurements may adversely affect the instrument's performance.

Details of all these features are provided in the "Windows Security" chapter of the [Keysight X-Series Signal Analyzer: Getting Started Guide](#).

Determining the Instrument's Operating System

You can easily determine your instrument's operating system version as follows:

1. Using the instrument front-panel, press **System > Control Panel...**
2. The Windows Control Panel appears. From the menu at the top of the Control Panel window, select **Help > About Windows**
3. The **About Windows** message box appears, displaying the installed version of Windows

USB Interfaces

The instrument's Microsoft Windows operating system can be configured to improve the security of the USB interfaces. This section includes the following topics:

["Disabling or Enabling AutoRun/AutoPlay" on page 48](#)

["Configuring USB for Read-only" on page 51](#)

Disabling or Enabling AutoRun/AutoPlay

AutoRun, and the associated AutoPlay, are Windows features that assist users in selecting appropriate actions when new media and devices are detected. The AutoRun feature is disabled in the instrument by default, for improved security, unless the Administrator account is running. (In Administrator mode, AutoRun is enabled, to aid with program installation.)

The procedure for disabling and enabling AutoPlay depends on your instrument's operating system (either [Windows 7](#) or [Windows XP](#)). To determine the operating system version of your instrument, see ["Determining the Instrument's Operating System" on page 48](#).

Windows 7

If your instrument has the Windows 7 operating system, you can disable or enable AutoPlay via the Control Panel. Open the Control Panel and select **Hardware and Sound > AutoPlay**, then uncheck or check the "Use AutoPlay for all media and devices" checkbox.

If you want to understand details of how this AutoPlay setting affects the Windows Registry, see the [Windows XP](#) discussion below.

Windows XP

You can change the AutoRun configuration by editing the value of one of two Windows Registry keys. The Windows Registry is a database that stores critical configuration information for the instrument's operating system.

CAUTION Exercise extreme caution whenever you edit the Windows Registry. Entering an incorrect Registry value, or accidentally deleting Registry keys, may have serious consequences that can prevent the system from starting, or require that you reinstall Windows. The instructions in ["Disable & Enable Procedure" on page 50](#) below assume that you are familiar with the use of the

Windows Registry Editor to modify Registry settings.

Registry Key Definitions

AutoRun can be configured per-machine or per-user.

NOTE If the per-machine Registry key is present, its settings override those of the per-user Registry key.

The Registry key that controls the **per-machine** AutoRun settings is:

`HKEY_LOCAL_MACHINE\Software\Microsoft\Windows\CurrentVersion\Policies\Explorer\NoDriveTypeAutoRun`


The Registry key that controls the **per-user** AutoRun settings is:

`HKEY_CURRENT_USER\SOFTWARE\Microsoft\Windows\CurrentVersion\policies\Explorer\NoDriveTypeAutoRun`

In the following discussions, we use the industry-standard abbreviation **HKLM** for the root key `HKEY_LOCAL_MACHINE`, and the industry-standard abbreviation **HKCU** for the root key `HKEY_CURRENT_USER`.

The **DWORD** value of either of these entries represents a set of single-bit flags. Each flag specifies the AutoRun setting for a specific drive type, as shown in [Figure 8-1](#). Setting a bit flag to 1 disables AutoRun for that drive type.

Figure 8-1 AutoRun Flag Definitions for NoDriveTypeAutoRun Registry entry

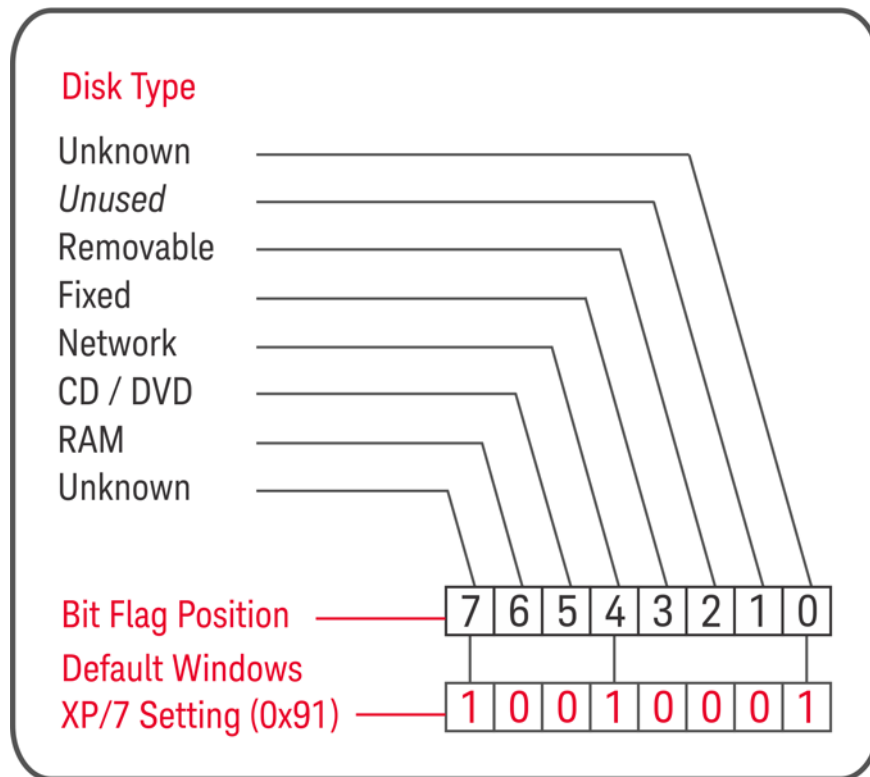

User and Remote Interface Security Measures

USB Interfaces

As shown in [Figure 8-1](#) above, the default Windows XP (post-SP2) and Windows 7 value for this entry is 0x91 (under the entry HKCU\...\NoDriveTypeAutoRun). This setting disables AutoRun for **Unknown** and **Network** drives, but enables AutoRun for **Removable**, **Fixed**, **CD/DVD** or **RAM** drives.

You can disable AutoRun for all drive types by changing the value to 0xFF, as described in the following section.


Disable & Enable Procedure

In view of the interaction between the per-machine and per-user Registry settings, as described above, it is recommended that, if both keys exist in your instrument's Registry, you should alter the settings of **both** Registry keys to the same value at the same time.

Use the following procedure to disable AutoRun for all drive types, or to revert all AutoRun settings to their Windows XP or Windows 7 default values. (Note that if your instrument has a Windows 7 operating system, there is a simpler way to do this via the Control Panel; see "[Windows 7](#)" on [page 48](#) above.)


1. Open the Windows Registry editor, using one of the following methods depending on your instrument's operating system:
 - a. For Windows XP, select **Run...** from the Windows Start menu. Then, type `regedit` into the Windows Run dialog box, as shown in [Figure 8-2](#) below, and click **OK**.

Figure 8-2 Windows XP Run Dialog

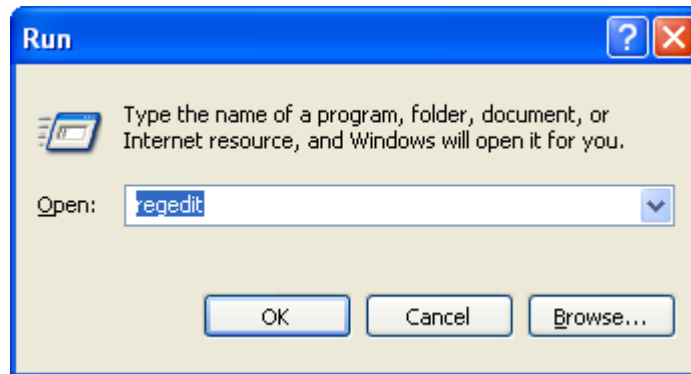

- b. For Windows 7, click the Windows **Start** button at the bottom left of the screen, type `regedit` into the **Search programs and files** box, as shown in [Figure 8-3](#) below, then press **Enter**.

Figure 8-3 Windows 7 Search edit box

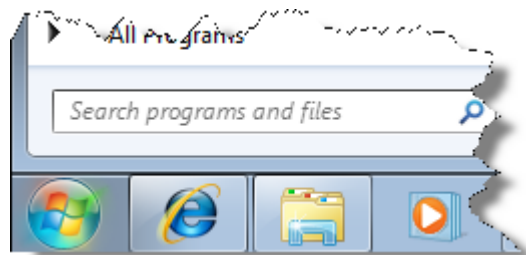

2. The Registry Editor window appears. Using the tree view control on the left of the window, navigate to the per-machine (HKLM) key: `HKLM\Software\Microsoft\Windows\CurrentVersion\Policies\Explorer`.
3. To **disable** AutoRun for all drive types, set the value of entry `NoDriveTypeAutoRun` to `0xff`.

To **revert** AutoRun settings to the Windows default values, set the value of entry `NoDriveTypeAutoRun` to `0x91`.

4. Again using the tree view control on the left of the Registry Editor window, navigate to the per-user (HKCU) key: `HKCU\SOFTWARE\Microsoft\Windows\CurrentVersion\Policies\Explorer`.
5. To **disable** AutoRun for all drive types, set the value of entry `NoDriveTypeAutoRun` to `0xff`.
To **revert** AutoRun settings to the Windows default values, set the value of entry `NoDriveTypeAutoRun` to `0x91`.
6. From the Registry Editor menu, select **File > Exit** to save the settings and exit the editor.
7. Shut down and restart the instrument, to enable the new settings to take effect.

Microsoft AutoRun Patch

NOTE The information in this section applies only to Windows XP. If your instrument has a Windows 7 operating system, you do not require this patch.

There is a defect in Windows XP that compromises the ability to disable AutoRun. This defect has been fixed by a patch from Microsoft, as described in the [Microsoft Knowledge Base Article ID: 967715](#).

This patch has been included in new instrument shipments from the factory since revision A.03.00.

After the patch has been applied, there will be a Registry entry at:

`HKLM\Software\Microsoft\Windows\CurrentVersion\Policies\Explorer\HonorAutorunSetting` with a default value of 1.

More Information

The following Wikipedia articles provide more information about AutoRun and AutoPlay:

<http://en.wikipedia.org/wiki/AutoRun>

<http://en.wikipedia.org/wiki/AutoPlay>

Configuring USB for Read-only

As from instrument software revision A.04.00, a convenient mechanism is provided to set the instrument's USB interfaces to read-only, thus preventing transfer of files from the instrument onto USB devices.

You can change this setting only when you are logged on as the Administrator. For details of how to log on to the instrument as the Administrator, see the [Keysight X-Series Signal Analyzer: Getting Started Guide](#). To change the setting, do the following:

1. If you are **not** currently logged on to the instrument as the Administrator, you must log off.
If you are currently logged on to the instrument as the Administrator, and the Keysight XSA application is already running, go to Step 4.
The log-off procedure executes more quickly if you first exit the Keysight XSA application, but you can also log off without exiting the application.
2. To log off, use one of the following procedures, depending on your instrument's operating system:
 - a. For Windows XP, select **Log Off** from the Windows XP Start menu (as highlighted in [Figure 8-4](#) below), then click **Log Off** in the Log Off Windows dialog that appears.

User and Remote Interface Security Measures


USB Interfaces

Figure 8-4 Log Off Button in Windows XP Start Menu



- b. For Windows 7, click the Windows **Start** button, then select **Shut down > Log off** from the Windows Start menu, as shown in [Figure 8-5](#) below.

Figure 8-5 Windows 7 Log off Control

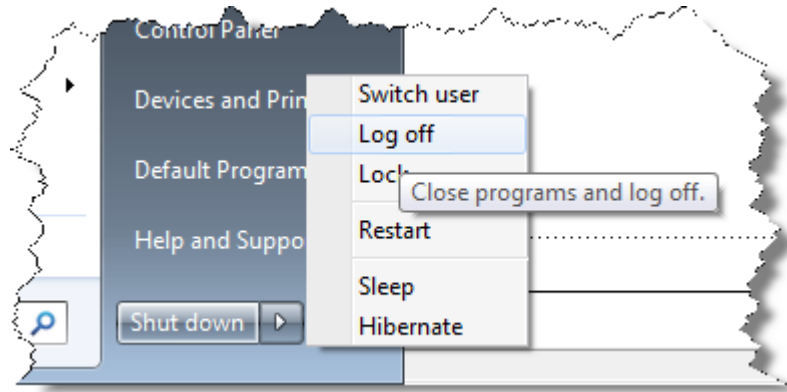

3. After you have logged on to the instrument as the Administrator, restart the Keysight XSA application.
4. When the XSA application has fully initialized (that is, when the main results view and softkey menu are visible), press the **System** front-panel key.
5. From the System softkey menu, select: **More > Security > USB**.
6. Select the option **Read Only**.
7. To activate the configuration change, either log out and then back in under your usual user name (which by default is "instrument"), or cycle the instrument power.

9 Procedure for Declassifying a Faulty Instrument

Even if the instrument is not able to power on, it may be declassified by removing the disk drive from the instrument, using the appropriate procedure as described in [“Disk Drive Removal Procedure”](#) on page 43.

Procedure for Declassifying a Faulty Instrument

10 Special Options

There are certain special options for X-Series instruments that provide security-related functionality. The following available options are described in this chapter.

- “Option SF1” on page 56
- “Option SF2” on page 57

Option SF1

Option SF1 is a license key-enabled special option that addresses the requirements of security-conscious users. Installing Option SF1 in the instrument causes changes to available functionality in certain menus, and suppression of certain SCPI commands, to prevent the launching of Windows programs from the instrument application. This reduces the instrument's vulnerability to the effects of unauthorized or undesirable third-party programs or scripts.

This section summarizes the functional modifications to the instrument capabilities when Option SF1 is installed.

Support

Option SF1 is supported on all X-Series instruments with software revision A.12.06 or greater.

Menu & Command Changes

Installing Option SF1 causes the following menu and command changes in the instrument.

File Menu

- In the **File** menu, the **File Explorer...** key is not available.

System Menu

- In the **System** menu, the keys **Control Panel...**, **Licensing...**, and **Internet Explorer...** are not available.
- In the **System > Diagnostics** menu, the keys **Front Panel Test...**, **Advanced**, **FP State Logger**, and **Quick Test...**, and the functions of all submenus of these keys, are not available.
- In the **System > Service > Diagnostics** menu, the **Advanced** key and all functions of its submenu are not available.
- In the **System > Service > Align > Diagnostics** menu, the **Align Log...** key is not available.

SCPI Commands

- The SCPI command `:SERVICE[:PRODUCTION]:RUN` is not available.

Right-Click (Popup) Menu

When Option SF1 is installed, the **Virtual Front Panel** selection and functionality (under the **Utility** menu) are not available.

Option SF2

Option SF2 is a license key-enabled special option that addresses the requirements of security-conscious users who need to be able to prevent the saving of measurement results or user configurations to the instrument's disk drive. The option also prevents the recall of results and configurations from the disk.

Installing Option SF2 makes the following changes to the instrument's operating environment:

- Modifies aspects of the Windows operating system, specifically to disable memory page file usage. For details, see ["Operating System Changes" on page 57](#).
- Disables certain menu keys and SCPI commands, eliminating the ability to save or recall user data. For details, see ["Menu & Command Changes" on page 58](#).

Support

Option SF2 is supported on all X-Series instruments with software revision A.14.00 or greater. This option requires the instrument to have the Windows 7 operating system. Instruments with the Windows XP operating system do not support Option SF2. (For more information, see ["Determining the Instrument's Operating System" on page 48](#).)

Operating System Changes

Installing Option SF2 disables Windows memory page files. The reason for this change is to ensure that memory page swapping does not inadvertently cause the instrument to create on-disk copies of RAM data.

Note that one effect of disabling memory page files is to reduce the available memory space for preloading applications at power-on.


TIP

If a disk recovery and software update to revision A.14.00 and above is performed, memory paging files will automatically be re-enabled. If the X-Series application is then started (with Option SF2 installed), the message shown in [Figure 10-1](#) appears, describing how to disable the page files.

The X-Series application will not start until memory page files are disabled. For details of how to run `SF2RegSetup.reg`, refer to [Installation Note: Keysight X-Series Signal Analyzers Option SF2](#).

Figure 10-1

Option SF2 System Incompatibility Message

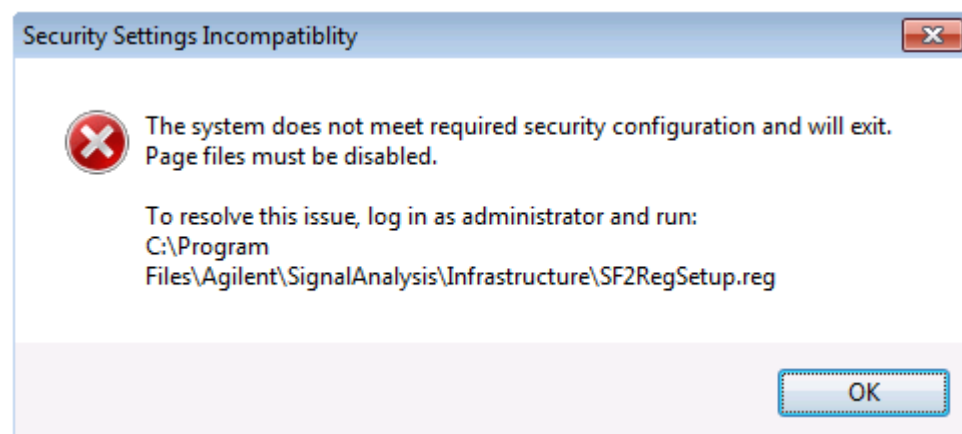

Menu & Command Changes

Installing Option SF2 causes several menu and command changes in the instrument, as follows.

Front-panel Keys

The functions of the following front-panel keys are disabled. Pressing one of these keys displays the informational message "Settings conflict; Feature not available for Option SF2".

- **Print**
- **Quick Save**
- **Recall**
- **Save**

NOTE Save and Recall are often used with the N9069A Noise Figure Measurement Application to allow multiple noise sources to be used without the need to re-enter ENR values or to perform the noise source calibration each time a different noise source is connected. When Option SF2 is installed, this functionality is not available.

File Menu

- The **Page Setup...** and **Print...** keys are not available.

System Menu

- In the **System > Power On** menu, the Power On Type selection keys (**Mode Preset**, **User Preset** and **Last State**) are not available.

SCPI Commands

The following SCPI commands are **not** available. Attempting to use these commands generates the Error message -113,"Undefined header".

Note that some of the commands listed are specific to individual applications, thus the set of available commands depends on which applications are licensed for a given instrument.

- *RCL
- *SAV
- :MMEMory:CLEar:ALL
- :MMEMory:CLEar:STATe
- :MMEMory:COMMeNt
- :MMEMory:COpy:DEvice
- :MMEMory:INITialize
- :MMEMory:LOAD:ALIMit
- :MMEMory:LOAD:ALISt
- :MMEMory:LOAD:ATRACE
- :MMEMory:LOAD:AUTO
- :MMEMory:LOAD:CAPTured
- :MMEMory:LOAD:CHTable

- :MMEMory:LOAD:CORRection
- :MMEMory:LOAD:ENR
- :MMEMory:LOAD:EVMSetup
- :MMEMory:LOAD:FREQuency
- :MMEMory:LOAD:LIMit
- :MMEMory:LOAD:LOSS
- :MMEMory:LOAD:MASK
- :MMEMory:LOAD:MPADapter:CORRection
- :MMEMory:LOAD:PSET
- :MMEMory:LOAD:REGister
- :MMEMory:LOAD:SCAN
- :MMEMory:LOAD:SETup
- :MMEMory:LOAD:SLISt
- :MMEMory:LOAD:SSSetup
- :MMEMory:LOAD:STATe
- :MMEMory:LOAD:STATe:VSA
- :MMEMory:LOAD:T2Config
- :MMEMory:LOAD:TMMConfig
- :MMEMory:LOAD:TRACe
- :MMEMory:LOAD:TRACe:DATA
- :MMEMory:LOAD:TRACe:REGister
- :MMEMory:LOAD:VSASetup
- :MMEMory:LOAD:ZMAP
- :MMEMory:MSIS
- :MMEMory:NAME
- :MMEMory:NFIGure:LOAD:ENR
- :MMEMory:NFIGure:LOAD:FREQuency
- :MMEMory:NFIGure:LOAD:LOSS
- :MMEMory:NFIGure:STORE:ENR
- :MMEMory:NFIGure:STORE:FREQuency
- :MMEMory:NFIGure:STORE:LOSS
- :MMEMory:REGister:STATe:LABel
- :MMEMory:RESuLts:CORRection:MODE
- :MMEMory:RESuLts:LIMits:MODE
- :MMEMory:RESuLts:OUTPut
- :MMEMory:RESuLts:SCAN
- :MMEMory:RESuLts:SCReen:THEME
- :MMEMory:RESuLts:SLISt
- :MMEMory:RESuLts:TRACe:DATA
- :MMEMory:RESuLts:TRACe:HEADer

Special Options

Option SF2

- :MMEMory:RESuLts:TRACe:SETTing
- :MMEMory:SElect[:ITEM]:ALL
- :MMEMory:SElect[:ITEM]:DEFault
- :MMEMory:SElect[:ITEM]:HWSettings
- :MMEMory:SElect[:ITEM]:LINES:ALL
- :MMEMory:SElect[:ITEM]:NONE
- :MMEMory:SElect[:ITEM]:SCData
- :MMEMory:SElect[:ITEM]:TRACe[:ACTive]
- :MMEMory:SElect[:ITEM]:TRANsducer:ALL
- :MMEMory:STORE:ALIMit
- :MMEMory:STORE:ALISt
- :MMEMory:STORE:ATRACE
- :MMEMory:STORE:CAPTured
- :MMEMory:STORE:CHTable
- :MMEMory:STORE:CORRection
- :MMEMory:STORE:ENR
- :MMEMory:STORE:FREQuency
- :MMEMory:STORE:LIMit
- :MMEMory:STORE:LOSS
- :MMEMory:STORE:MPADapter:CORRection
- :MMEMory:STORE:PSET
- :MMEMory:STORE:RESuLts
- :MMEMory:STORE:RESuLts:MTABLE
- :MMEMory:STORE:RESuLts:PTABLE
- :MMEMory:STORE:RESuLts:SNGLS
- :MMEMory:STORE:RESuLts:SPECTrogram
- :MMEMory:STORE:SCAN
- :MMEMory:STORE:SCReen
- :MMEMory:STORE:SCReen:THEMe
- :MMEMory:STORE:SLISt
- :MMEMory:STORE:STATe
- :MMEMory:STORE:T2Config
- :MMEMory:STORE:TMMConfig
- :MMEMory:STORE:TRACe
- :MMEMory:STORE:TRACe:DATA
- :MMEMory:STORE:TRACe:REGISter
- :MMEMory:STORE:ZMAP
- :MMEMory:TRACe:CLIEnt
- :MMEMory:TRACe:CLIEnt:STATe
- :MMEMory:TRACe:OPERator

- :MMEMory:TRACe:OPERator:STATe
- :MMEMory:TRACe:PDEscription
- :MMEMory:TRACe:PDEscription:STATe
- :MMEMory:TRACe:TITLe
- :MMEMory:TRACe:TITLe:STATe
- :SYSTem:PON:TYPE
- :SYSTem:PRESet:SAVE
- :SYSTem:PRESet:TYPE
- :SYSTem:PRESet:USER
- :SYSTem:PRESet:USER:ALL
- :SYSTem:PRESet:USER:SAVE
- :SYSTem:PRINT:THEMe

Right-Click (Popup) Menu

When Option SF2 is installed, the following functionality is not available.

In the main menu:

- User Preset

Under the **Utility** submenu:

- Quick Save
- Save
- Recall

Special Options
Option SF2

A: References

- DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”**
United States Department of Defense. Revised February 28, 2006.
May be downloaded in Acrobat (PDF) format from:
http://www.dss.mil/isp/fac_clear/download_nispom.html
- ISFO Process Manual for the Certification and Accreditation of Classified Systems under the NISPOM**
Defense Security Service.
DSS-cleared industries may request a copy of this document via email, by following the instructions at:
<http://www.dss.mil/isp/odaa/request.html>
- Keysight X-Series Signal Analyzer: Getting Started Guide**
Keysight Technologies 2008-2014. Part Number: subject to change as document is revised.
A printed copy of this document is supplied with each Keysight X-Series Analyzer.
It is also available in Acrobat (PDF) form:

 - on the Documentation DVD supplied with each instrument,
 - on the instrument's disk drive at the following location:
C:\Program Files\Agilent\SignalAnalysis\Infrastructure\Help\bookfiles\getstart.pdf
 - via download from:
www.keysight.com/find/xseries_getting_started_guide
- Microsoft Knowledge Base Article ID: 967715**
"How to disable the AutoRun functionality in Windows": may be viewed at:
<http://support.microsoft.com/kb/967715>
Note that a second article, at: <http://support.microsoft.com/kb/953252>, "How to correct 'disable AutoRun registry key' enforcement in Windows", redirects to article ID 967715.
- Installation Note: Keysight X-Series Signal Analyzers Option SF2**
Keysight Technologies 2014. Part Number: N9020-90234.
May be downloaded from:
<http://literature.cdn.keysight.com/litweb/pdf/N9020-90234.pdf>

References