

CLOCK RM

7/4/72

Bob Hogarth

(keep)

From Carl Chestnut - 63



HEWLETT-PACKARD COMPANY

103AR
QUARTZ OSCILLATOR

THIS MANUAL COVERS A
SPECIAL MODIFICATION
OF THE INSTRUMENT.
SEE INSIDE COVER



OPERATING AND SERVICING MANUAL

FOR

SPECIFICATION H02-103A/AR

QUARTZ OSCILLATOR

Specification H02-103A/AR is a standard ^{hp} Model 103A/AR Quartz Oscillator in which a special 1.00273791 MC crystal has been installed.

This special instrument has the following Overall Stability Specifications;

Long-Term: 2 parts in 10^9 per day. Short-Term: Better than 5 parts in 10^{10} averaged over 1 second intervals.

In all other respects this instrument is electrically identical to the standard ^{hp} Model 103A/AR Quartz Oscillator and the information in the Operating and Service Manual for the standard instrument applies to this special instrument.

Encl:

103A

maa
362



OPERATING AND SERVICE MANUAL

MODEL 103AR

SERIALS PREFIXED: 135 -

**QUARTZ
OSCILLATOR**

Copyright HEWLETT-PACKARD COMPANY 1961
1501 PAGE MILL ROAD, PALO ALTO, CALIFORNIA, U.S.A.



TABLE OF CONTENTS

Section	Title	Page	Section	Title	Page
I	GENERAL INFORMATION	1-1	VI	TROUBLESHOOTING	6-1
1-1.	Introduction	1-1	6-1.	General Information	6-1
1-3.	Description	1-1	6-4.	Test Equipment	6-1
II	PREPARATION FOR USE	2-1	6-6.	Sectionalization	6-1
2-1.	Unpacking and Mechanical Inspection	2-1	6-9.	Localization	6-1
2-3.	Packing for Storage or Reshipment	2-1	VII	REPAIRS	7-1
2-5.	Environmental Conditions During Storage and Shipment	2-1	7-1.	Sections Requiring Special Attention	7-1
2-7.	Installation	2-1	7-2.	Oscillator Oven	7-1
2-12.	Starting the Regenerative Frequency Divider	2-1	7-5.	Transistors Q102, Q103, and Components	7-1
III	OPERATING INSTRUCTIONS	3-1	7-7.	Transistors Q201, Q202, Q205, Q207, and Components	7-2
3-1.	Power Supply	3-1	7-10.	Transistors Q102, Q103, Q104, and Components	7-2
3-3.	Front-Panel Controls	3-1	7-12.	Transistor and Components Replacement	7-2
3-5.	Output Connectors	3-1	7-16.	Output Signal Loading	7-2
3-7.	Oven Temperature and Stability	3-1	7-18.	Capacitor C117 Replacement	7-2
3-10.	Fine Frequency Adjustment	3-1	7-20.	Resistor R308 Replacement	7-2
3-13.	Coarse Frequency Adjustment	3-1	VIII	TESTING AND ADJUSTMENT	8-1
IV	PERIODIC INSPECTION AND MAINTENANCE		8-1.	Performance Check	8-1
4-1.	Daily Inspection	4-1	8-3.	Circuits Requiring Adjustment	8-1
4-3.	Maintenance	4-1	8-5.	Adjustments	8-1
V	PRINCIPLES OF OPERATION	5-1	8-6.	Amplifier Q103 and Q104 Neutralization	8-1
5-1.	Introduction	5-1	8-7.	Tuned Amplifier Q201	8-1
5-3.	Simplified Block Diagram	5-1	8-8.	Tuned Amplifier Q202	8-1
5-5.	Oscillator Oven	5-1	8-9.	Tuned Amplifier Q203	8-1
5-13.	1 mc Oscillator and Amplifiers	5-2	8-10.	Regenerative Divider Q204, Q205	8-1
5-16.	Regenerative Frequency Divider and 100 kc Amplifiers	5-2	8-11.	Oven Control Adjustment	8-1
5-21.	Power Supply (Regulator)	5-2	IX	REPLACEABLE PARTS	9-1
			9-1.	Introduction	9-1
			9-4.	Ordering Information	9-1


LIST OF ILLUSTRATIONS

Number	Title	Page	Number	Title	Page
1-1.	Model 103AR Quartz Oscillator . . .	1-1	7-1.	Bottom View Model 103AR	7-0
2-1.	Rear View Model 103AR	2-0	7-2.	Top View Model 103AR	7-1
3-1.	Front View Model 103AR	3-0	8-1.	Sample Curve	8-2
5-1.	Simplified Block Diagram	5-0	8-2.	Oscillator (Schematic)	8-3
5-2.	Functional Diagram	5-3	8-3.	Output (Schematic)	8-5
			8-4.	Oven Control (Schematic)	8-7

LIST OF TABLES

Number	Title	Page
1-1.	Specifications	1-0
6-1.	Circuit Check Meter Indications	6-1
8-1.	Circuits Requiring Adjustment	8-2
9-1.	Reference Designator to Stock Number	9-1
9-2.	Electrical Components	9-5
9-3.	Miscellaneous Components	9-10

Table 1-1. Specifications

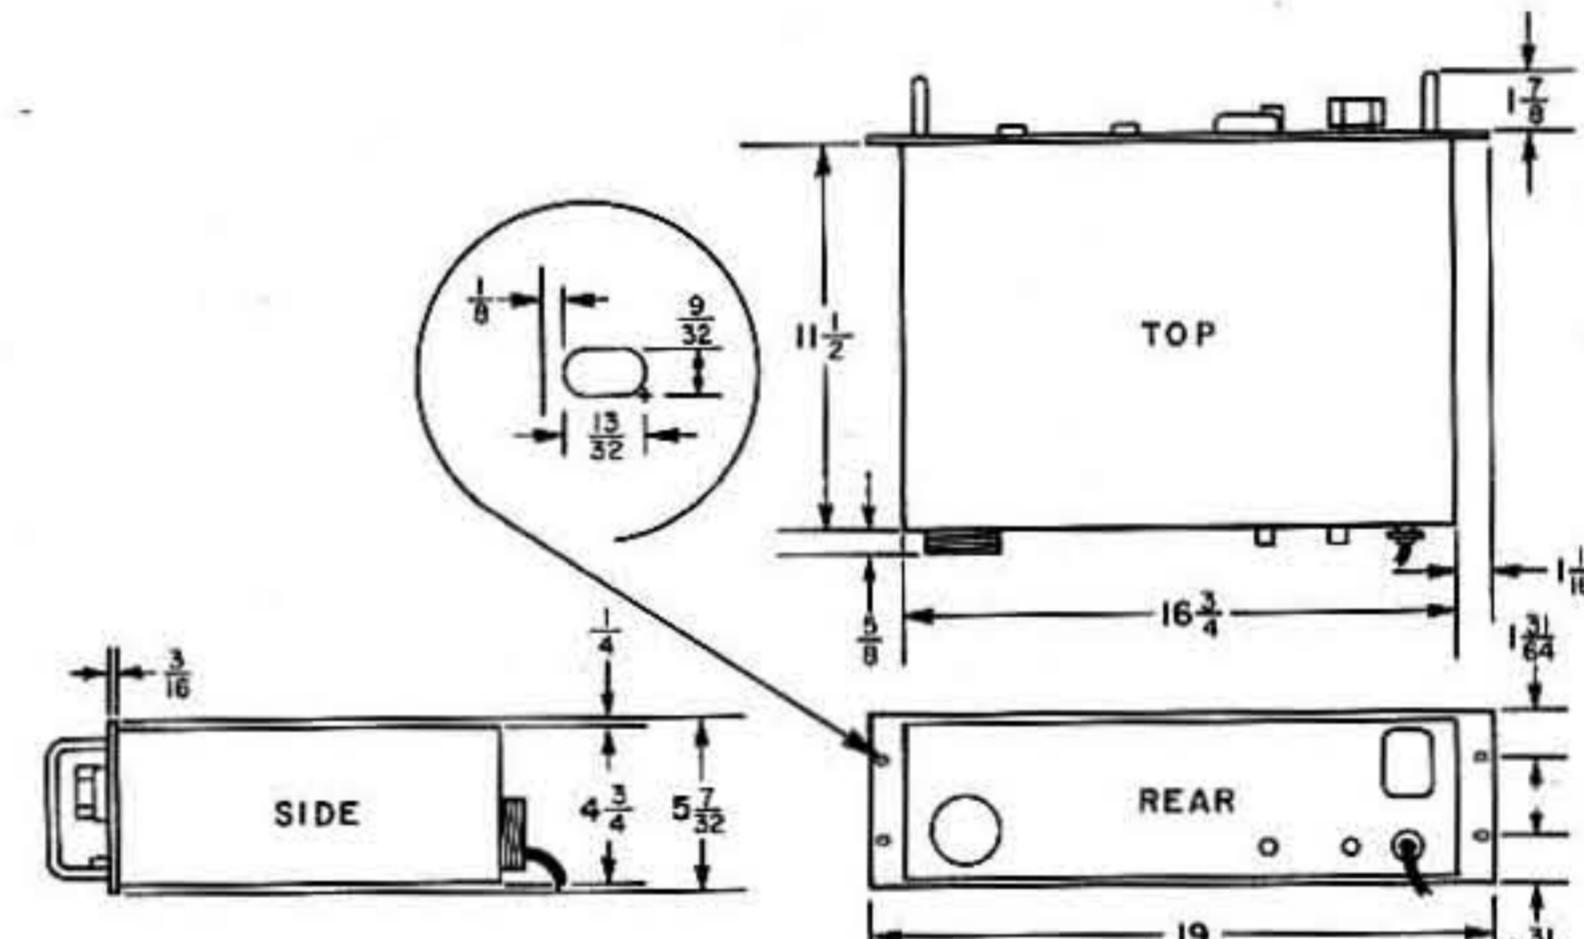AGING RATE: (after 21 days of operation)	$< \pm 5$ parts in 10^{10} per 24 hours*
STABILITY:	As a function of input voltage: $< \pm 1$ part in 10^{10} for changes of ± 4 volts from 26 volts dc As a function of load: $< \pm 1$ part in 10^{10} for changes from 50 ohms to open or short circuit As a function of ambient temperature: $< \pm 3$ part in 10^{10} for changes of $\pm 25^\circ\text{C}$ from 25°C
OUTPUT FREQUENCIES:	1) 1 mc sine waves, 1 volt rms into 50 ohms 2) 100 kc sine waves, 1 volt rms into 50 ohms 3) 100 kc output for driving $\text{\textcircled{H}}$ 113 Frequency Divider and Clock
HARMONIC DISTORTION:	At least 40 db below rated output
NON-HARMONICALLY RELATED OUTPUT:	At least 80 db below rated output
OUTPUT TERMINALS:	Outputs 1 and 2: BNC connectors on front panel and at rear Output 3: BNC connector at rear
FREQUENCY ADJUSTMENTS:	Coarse: Screwdriver adjustment with range of approximately 1 part in 10^6 . Accessible through front panel by removing threaded plug. Fine: Front-panel control with range of approximately 600 parts in 10^{10} . Accessible through front panel by removing threaded plug. Digital indicator calibrated directly in parts in 10^{10} .
MONITOR METER:	Ruggedized front-panel meter and associated selector switch monitors: 1) SUPPLY voltage 4) OUTER OVEN current 2) OSC voltage 5) 1 MC output 3) INNER OVEN current 6) 100 KC output
TEMPERATURE RANGE:	0-50°C
SIZE:	Rack Mount: 
WEIGHT:	Net approximately 17 lbs
POWER REQUIREMENT:	22 to 30 volts dc positive ground, approximately 5 watts after warmup at room temperature. Approximately 10 watts maximum during warmup. $\text{\textcircled{H}}$ 724BR/725AR Standby Power Supply with standby battery recommended.
ACCESSORY FURNISHED:	Cable for connecting $\text{\textcircled{H}}$ 103AR Frequency Standard to $\text{\textcircled{H}}$ Standby Power Supply
COMPLEMENTARY EQUIPMENT:	$\text{\textcircled{H}}$ Model 724BR Standby Power Supply, with battery, 16 ampere-hour standby capacity $\text{\textcircled{H}}$ Model 725AR Standby Power Supply with battery, 2 ampere-hour capacity $\text{\textcircled{H}}$ Model 113BR Frequency Divider and Clock $\text{\textcircled{H}}$ Model 120AR Oscilloscope

SECTION I

GENERAL INFORMATION

1-1. INTRODUCTION.

1-2. This manual provides instructions on installation, operation, and maintenance of the **hp** Model 103AR Quartz Oscillator, and applies directly to all instruments whose serial number is prefixed as indicated on the title page. The serial number is stamped on the tag at the rear of the chassis.

1-3. DESCRIPTION.

1-4. The **hp** 103AR Quartz Oscillator has a stability of 5 parts in 10^{10} per day or better. High stability is achieved by housing the high-quality crystal and all critical elements in a double oven having proportional control. Short-term stability is 5 parts in 10^{10} averaged over one-second intervals. Under reasonably constant conditions, short-term stability is typically one part in 10^{10} averaged over one second intervals.

1-5. The oscillator is well isolated from external circuit influences. Each output signal is isolated in such a way that short-circuiting the 1-mc output will not affect the 100-kc output and vice versa.

1-6. Two output signals, 1 mc and 100kc are supplied from a low impedance source at a power level well suited for distribution over 50-ohm systems. A

separate 100-kc output signal is furnished for driving the 113AR/BR Frequency Divider and Clock or equivalent. Fail-safe operation is provided by using a non-selfstarting regenerative frequency divider. The 100-kc output will cease if any interruptions of power or signal occur.

1-7. The 103AR Quartz Oscillator is used in primary frequency and time standards. The **hp** 103AR Quartz Oscillator, **hp** 724BR Standby Power Supply, and **hp** 113AR/BR Frequency Divider and Clock are the basic elements of a primary frequency and time standard system of small size, and capable of high resolution accuracy. For high frequency (hf) time comparisons, a receiver and triggered oscilloscope such as the **hp** Model 120AR complete the system. Very low frequency (vlf) comparisons may be made by using a time interval counter such as the **hp** Model 523 or 524 series electronic counters. Power for the Model 103AR can be obtained from the Model 724BR. Power interruptions have no effect on performance. For use as a secondary standard, only the 103AR and 724BR are required.

1-8. Throughout this manual, the AR Quartz Oscillator will be referred to as the "oscillator", and the 113AR/BR Frequency Divider and Clock will be referred to as the "clock".

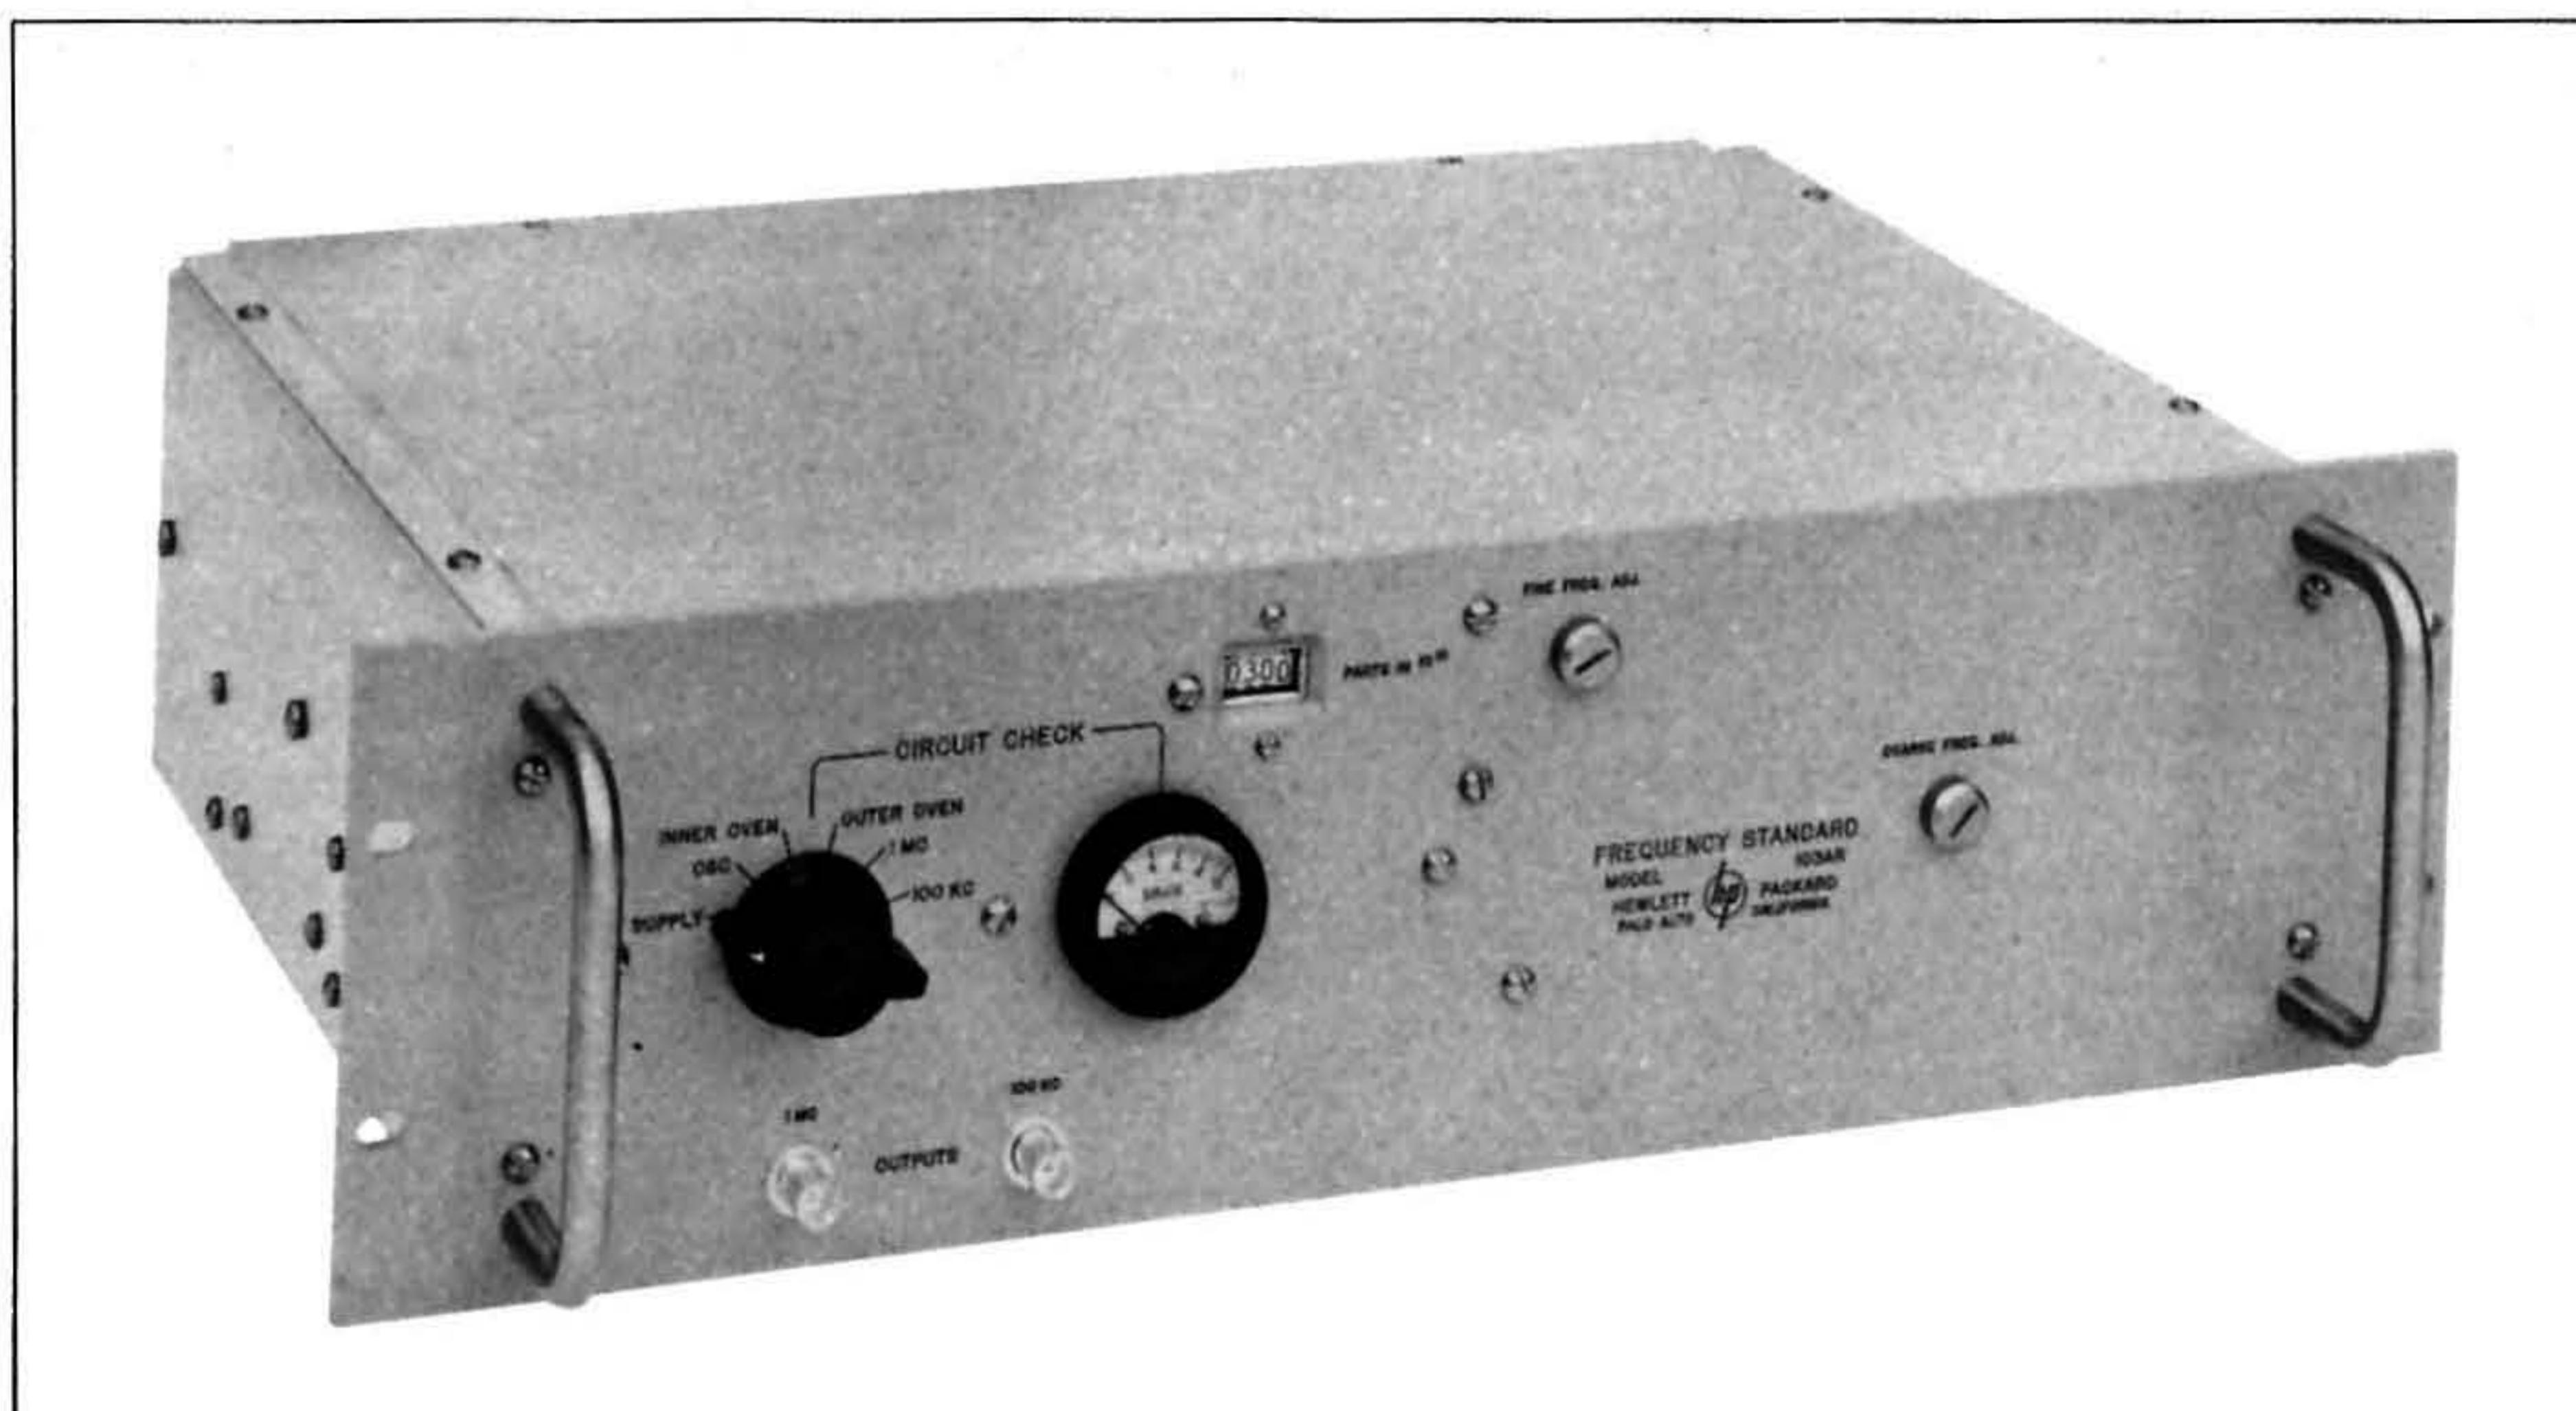


Figure 1-1. Model 103AR Quartz Oscillator

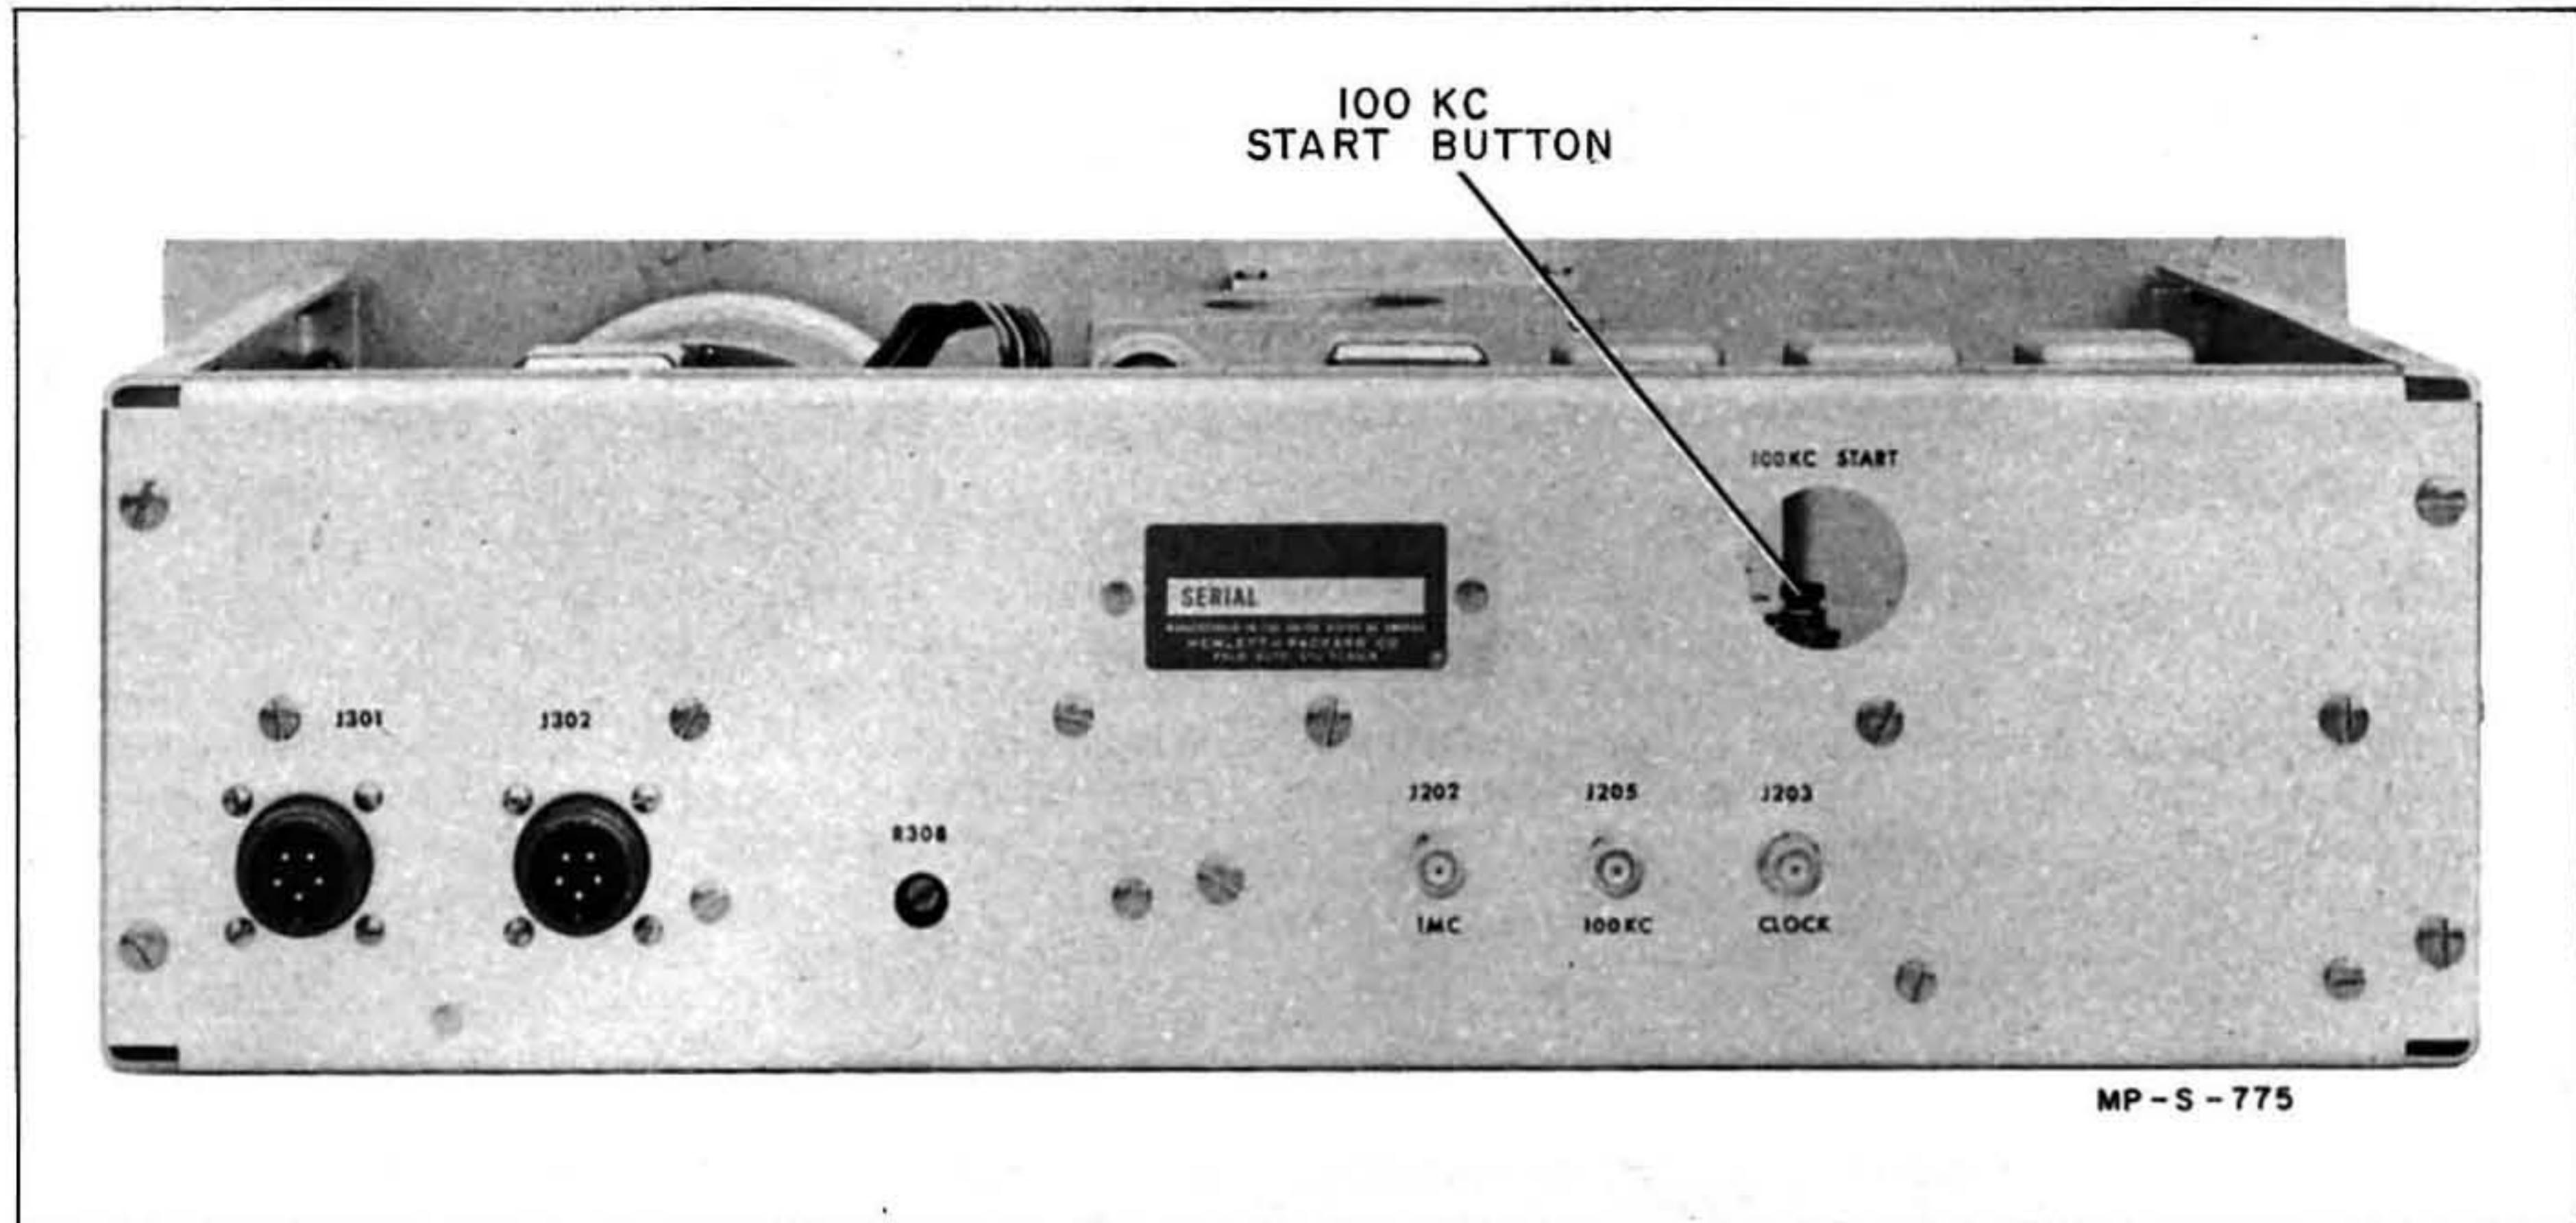


Figure 2-1. Rear View Model 103AR

SECTION II

PREPARATION FOR USE

2-1. UNPACKING & MECHANICAL INSPECTION.

2-2. Inspect the instrument for shipping damage as soon as it is unpacked. If reshipment is expected, save all packing material. Check for broken knobs, meter faces, or connectors. Inspect painted surfaces for scratched or abraded areas. If the instrument is damaged in any way, notify the carrier to report damage immediately. Carrier will arrange for repair or reshipment as necessary.

2-3. PACKING FOR STORAGE OR RESHIPMENT.

2-4. To protect valuable electronic equipment during storage or shipment, always use the best packaging methods available. Contract packaging companies in many cities can provide dependable packing on short notice. The following packaging methods are recommended:

a. Original. Place instrument in original container. Replace all packing pads and fillers in the exact position they originally occupied.

b. Rubberized Hair. Cover painted surfaces of instrument with protective wrapping paper. Pack instrument securely in strong corrugated container (350 lb/square inch bursting test) with 2-inch rubberized hair pads placed along all surfaces of the instrument. Insert filler between pads and container to insure a snug fit on all surfaces of the instrument.

c. Excelsior. Cover painted surfaces with protective wrapping paper. Pack instrument in a strong corrugated container (350 lb/square inch bursting test) with a layer of excelsior about 6 inches thick, packed firmly against all surfaces of the instrument.

2-5. ENVIRONMENTAL CONDITIONS DURING STORAGE AND SHIPMENT.

2-6. Environmental conditions during storage and shipment should normally be limited as follows:

- a. Maximum altitude: 20,000 feet.
- b. Maximum temperature: 65°C (144°F).
- c. Minimum temperature: -40°C (-40°F).

2-7. INSTALLATION.

WARNING

If the oscillator is being used with a clock, the clock must have a positive ground. The oscillator uses a positive ground. If the clock has a negative ground and the oscillator is connected to the system, a short circuit will exist. Use an isolated power supply for oscillator or change the clock to use a positive ground.

2-8. Mount the oscillator in a standard size rack. Ambient temperature in the rack during operation should not exceed a maximum of 50°C (122°F) or a minimum of 0°C (32°F).

2-9. Connect the socket end of the power cable (supplied with the oscillator) to either of the power connectors, J301 or J302, at the rear of the instrument. Pin A of either connector must be connected to the positive terminal of the dc supply. Pin C must be connected to the negative terminal of the dc supply.

2-10. Set the CIRCUIT CHECK switch to SUPPLY. The meter should indicate between 7.0 and 9.0.

2-11. If the oscillator is not used with the clock, connect the appropriate output of the oscillator to input of the system used. If the oscillator is to be used with the clock, connect the clock 100 KC INPUT connector to the CLOCK connector at the rear of the oscillator. The oscillator has been adjusted at the factory for optimum performance and should require no adjustment.

- a. OSC: Meter should indicate between 7.0 and 9.0.
- b. INNER OVEN: Same as step a (7.0 and 9.0).
- c. OUTER OVEN: Meter may indicate between 7.0 and 10.0, depending upon the oven temperature.
- d. 100 KC: Meter should indicate zero.
- e. 1 MC: Meter should indicate between 7.0 and 9.0.

2-12. STARTING THE REGENERATIVE FREQUENCY DIVIDER.

2-13. To start the regenerative frequency divider, depress the 100 KC START button. See figure 2-1. After the button is depressed, set the CIRCUIT CHECK switch to 100 KC. The meter should indicate between 7.0 and 9.0.

2-14. If the oscillator is being used with the clock, start the clock. Refer to the clock manual. If the clock does not start, check the oscillator. See section VIII of this manual. If it is determined the oscillator is operating properly, troubleshoot the clock.

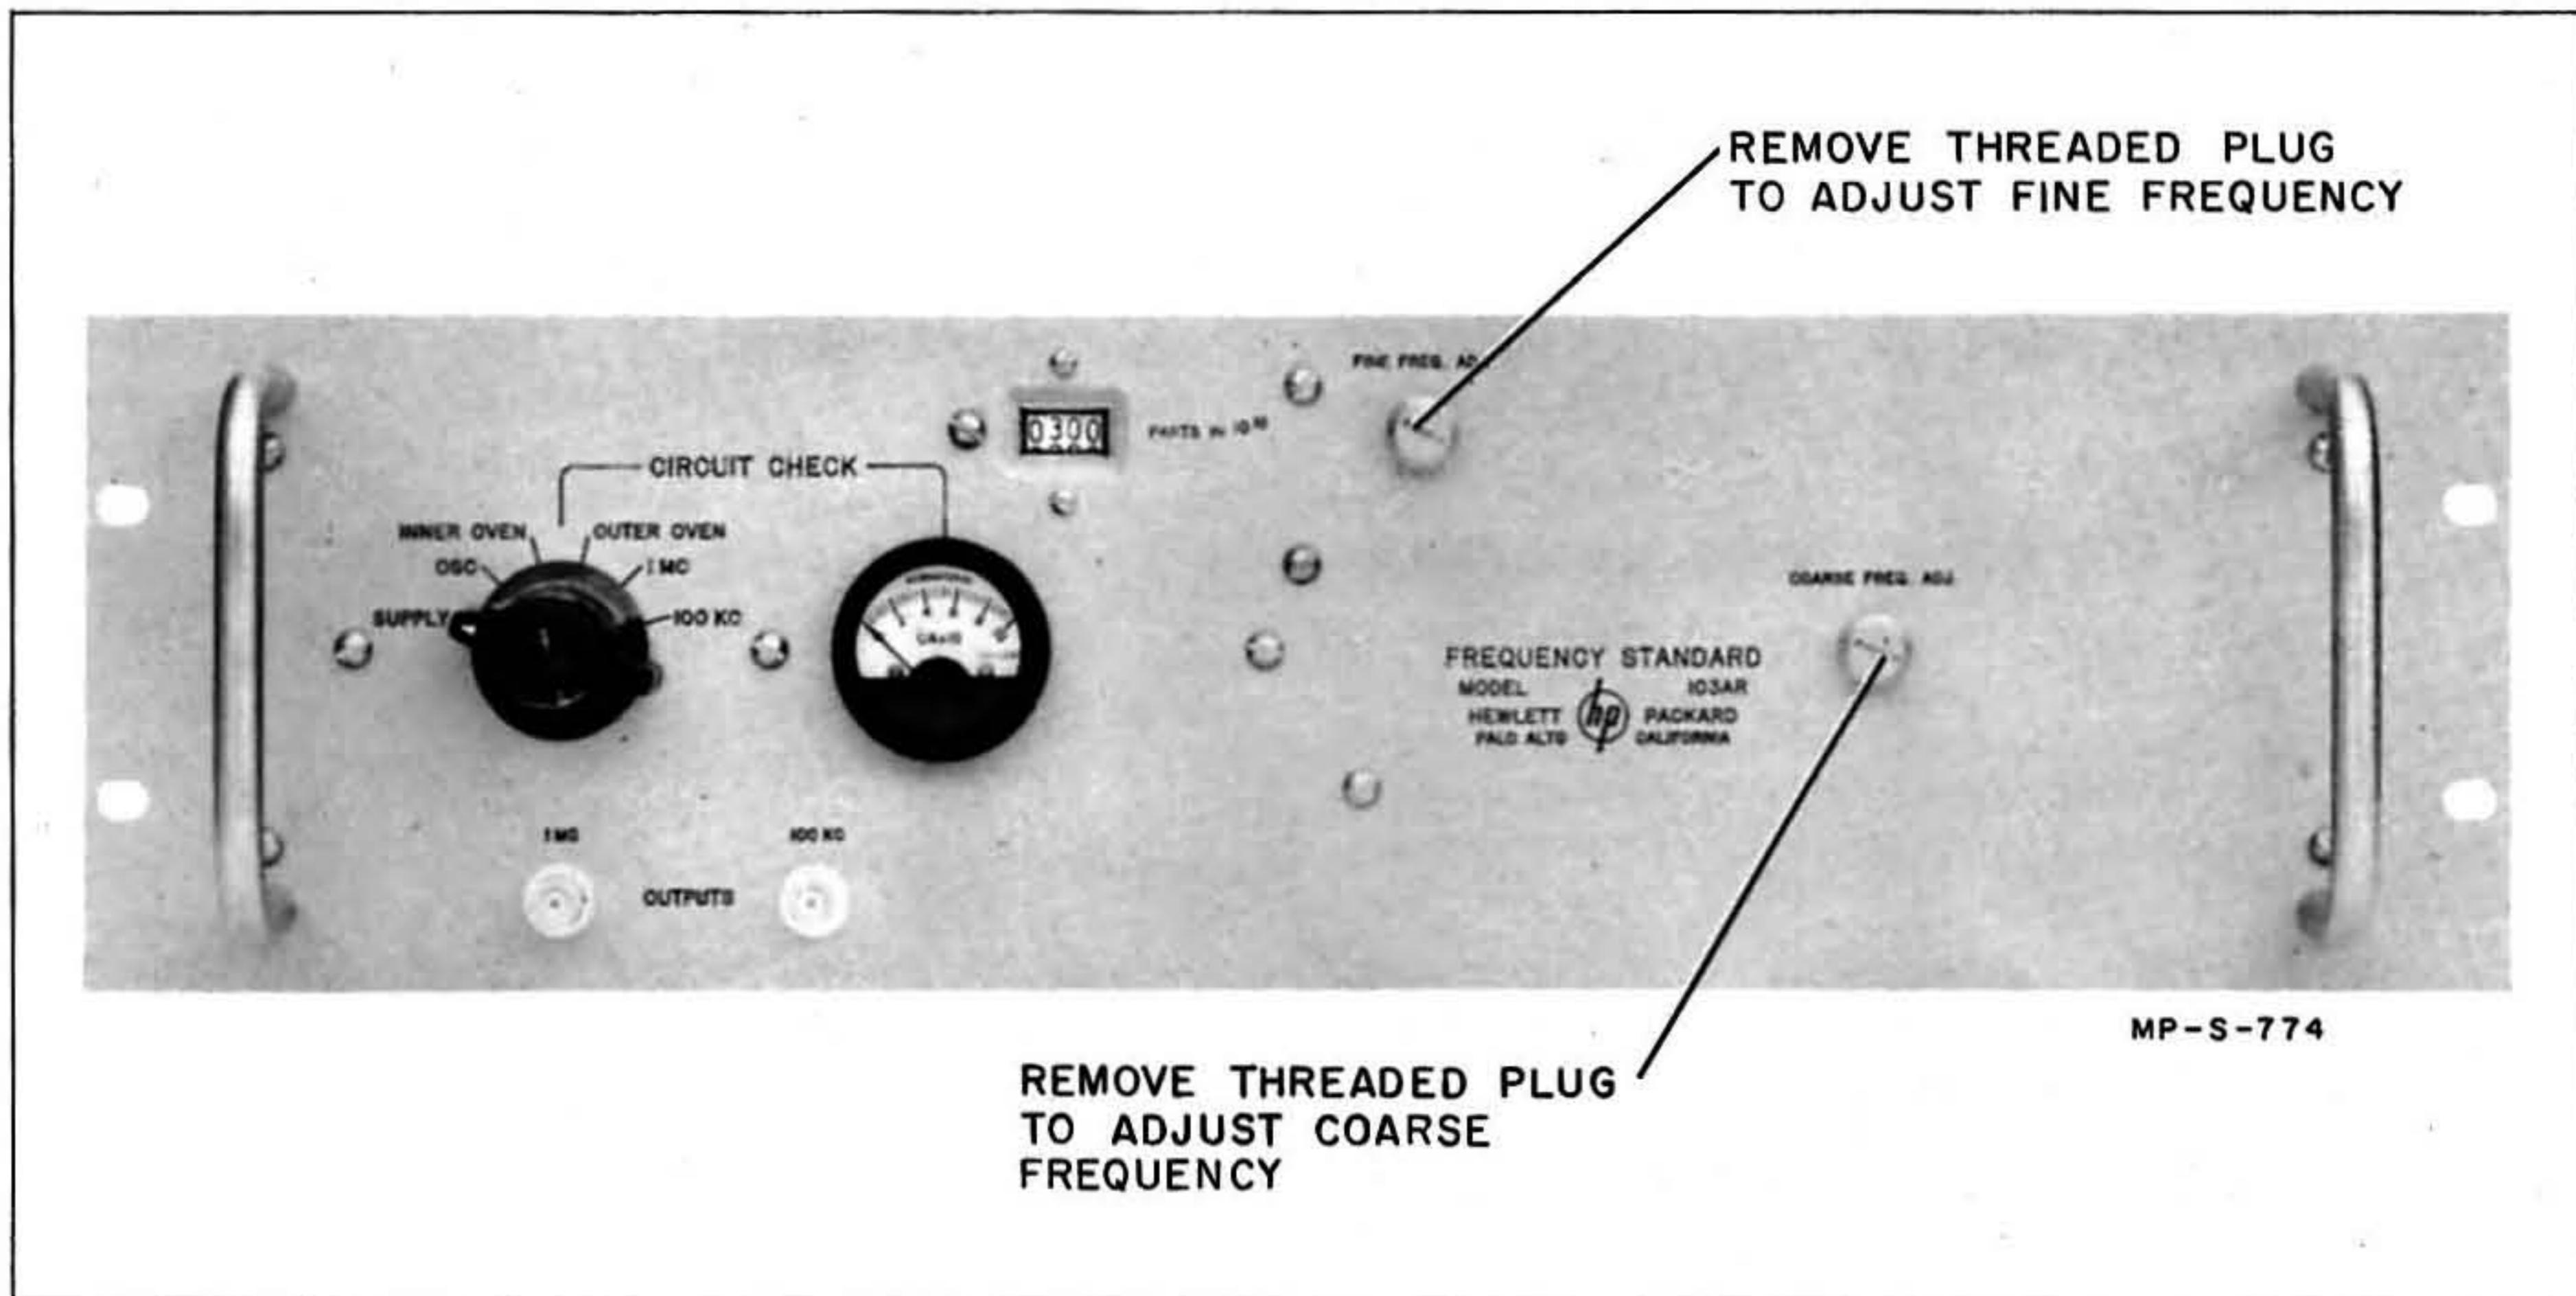


Figure 3-1. Front View Model 103AR

SECTION III

OPERATING INSTRUCTIONS

3-1. POWER SUPPLY.

3-2. Power is supplied to the oscillator immediately when the power cable is connected to the 724BR power supply or equivalent. The oscillator is not equipped with a power on-off switch. To remove power from the oscillator, disconnect the power connector from the rear of the instrument.

3-3. FRONT-PANEL CONTROLS.

3-4. The oscillator has three front-panel controls (see figure 3-1):

- a. CIRCUIT CHECK switch: Enables the operator to monitor the operation of various circuits.
- b. FINE FREQ. ADJ.: Available from the front panel when the threaded plug is removed. The control is geared to the PARTS IN 10^{10} counter and gives a visual indication as FINE FREQ. ADJ. is turned.
- c. COARSE FREQ. ADJ.: Available from the front panel when the threaded plug is removed. Gives a larger change of frequency with no visual indication.

3-5. OUTPUT CONNECTORS.

3-6. The oscillator has five signal output connectors. The front panel has two output connectors, 100 KC and 1 MC OUTPUTS (see figure 3-1). The rear of the instrument has three output connectors, 100 KC, 1 MC, and CLOCK. The front panel 100 KC and 1 MC OUTPUTS are parallel with the rear 100 KC and 1 MC outputs (see figures 2-1 and 3-1).

3-7. OVEN TEMPERATURE AND STABILITY.

3-8. After the oscillator is initially connected to power, three weeks may be required for the crystal to stabilize to 5 parts in 10^{10} .

3-9. The oven is held to within approximately 1/500 of a degree. When the oscillator is tested at the factory, the oven is adjusted to the temperature of maximum stability of the individual crystal. As the oven temperature is varied, the oscillator frequency will vary as shown in figure 8-1.

NOTE

The operating point of the oven is set at the factory and cannot be changed unless another frequency standard with stability equal to or better than the oscillator is available. Under these conditions the operating point can be changed. See paragraph 8-11.

3-10. FINE FREQUENCY ADJUSTMENT.

3-11. The FINE FREQ. ADJ. is geared to the PARTS IN 10^{10} counter. As the FINE FREQ. ADJ. is turned, the counter registers the frequency change in the number of parts in 10^{10} . The counter is usable only to 600. After 600 the hundreds digit appears in red. When the red number is reached, it becomes necessary to use the COARSE FREQ. ADJ. (paragraph 3-13).

3-12. After the oscillator has stabilized, periodic corrections will be necessary. If the oscillator is used with the clock, when a time comparison is made, the time the clock has gained or lost divided by the period between measurements, in seconds, will give the oscillator error in 10^{10} . The PARTS IN 10^{10} counter is then advanced or retarded by turning the FINE FREQ. ADJ. For additional information see the ^{hp} Application Note 52, available from the Hewlett-Packard Company.

3-13. COARSE FREQUENCY ADJUSTMENT.

3-14. If it is necessary to set the COARSE FREQ. ADJ. proceed as follows:

- a. Remove the COARSE FREQ. ADJ. threaded plug on front panel. The COARSE FREQ. ADJ. gives 10,000 parts in 10^{10} change for approximately 180° rotation, thus 180° rotation will give approximately 1000 parts in 10^{10} change, and $4-1/2^\circ$ will give approximately 250 parts in 10^{10} change.
- b. Remove the FINE FREQ. ADJ. threaded plug. Adjust the FINE FREQ. ADJ. until the PARTS IN 10^{10} counter indicates 300.
- c. Adjust the COARSE FREQ. ADJ. clockwise, $4-1/2^\circ$ for a frequency higher by 250 parts in 10^{10} , or counterclockwise $4-1/2^\circ$ for a frequency lower by 250 parts in 10^{10} . Adjustment is made by inserting a screwdriver in the COARSE FREQ. ADJ., pressing in and turning the screwdriver until the outer shaft becomes engaged with the COARSE FREQ. ADJ. capacitor shaft. Then adjust as needed.
- d. Replace the COARSE and FINE FREQ. ADJ. threaded plugs.
- e. The accuracy of the adjustment can be determined when the next time comparison measurement is made. Use the average of several time comparison measurements taken several days apart to adjust any error out of the oscillator.
- f. If the oscillator is still out of the range of the FINE FREQ. ADJ., repeat steps b through e.
- g. Replace threaded plugs.

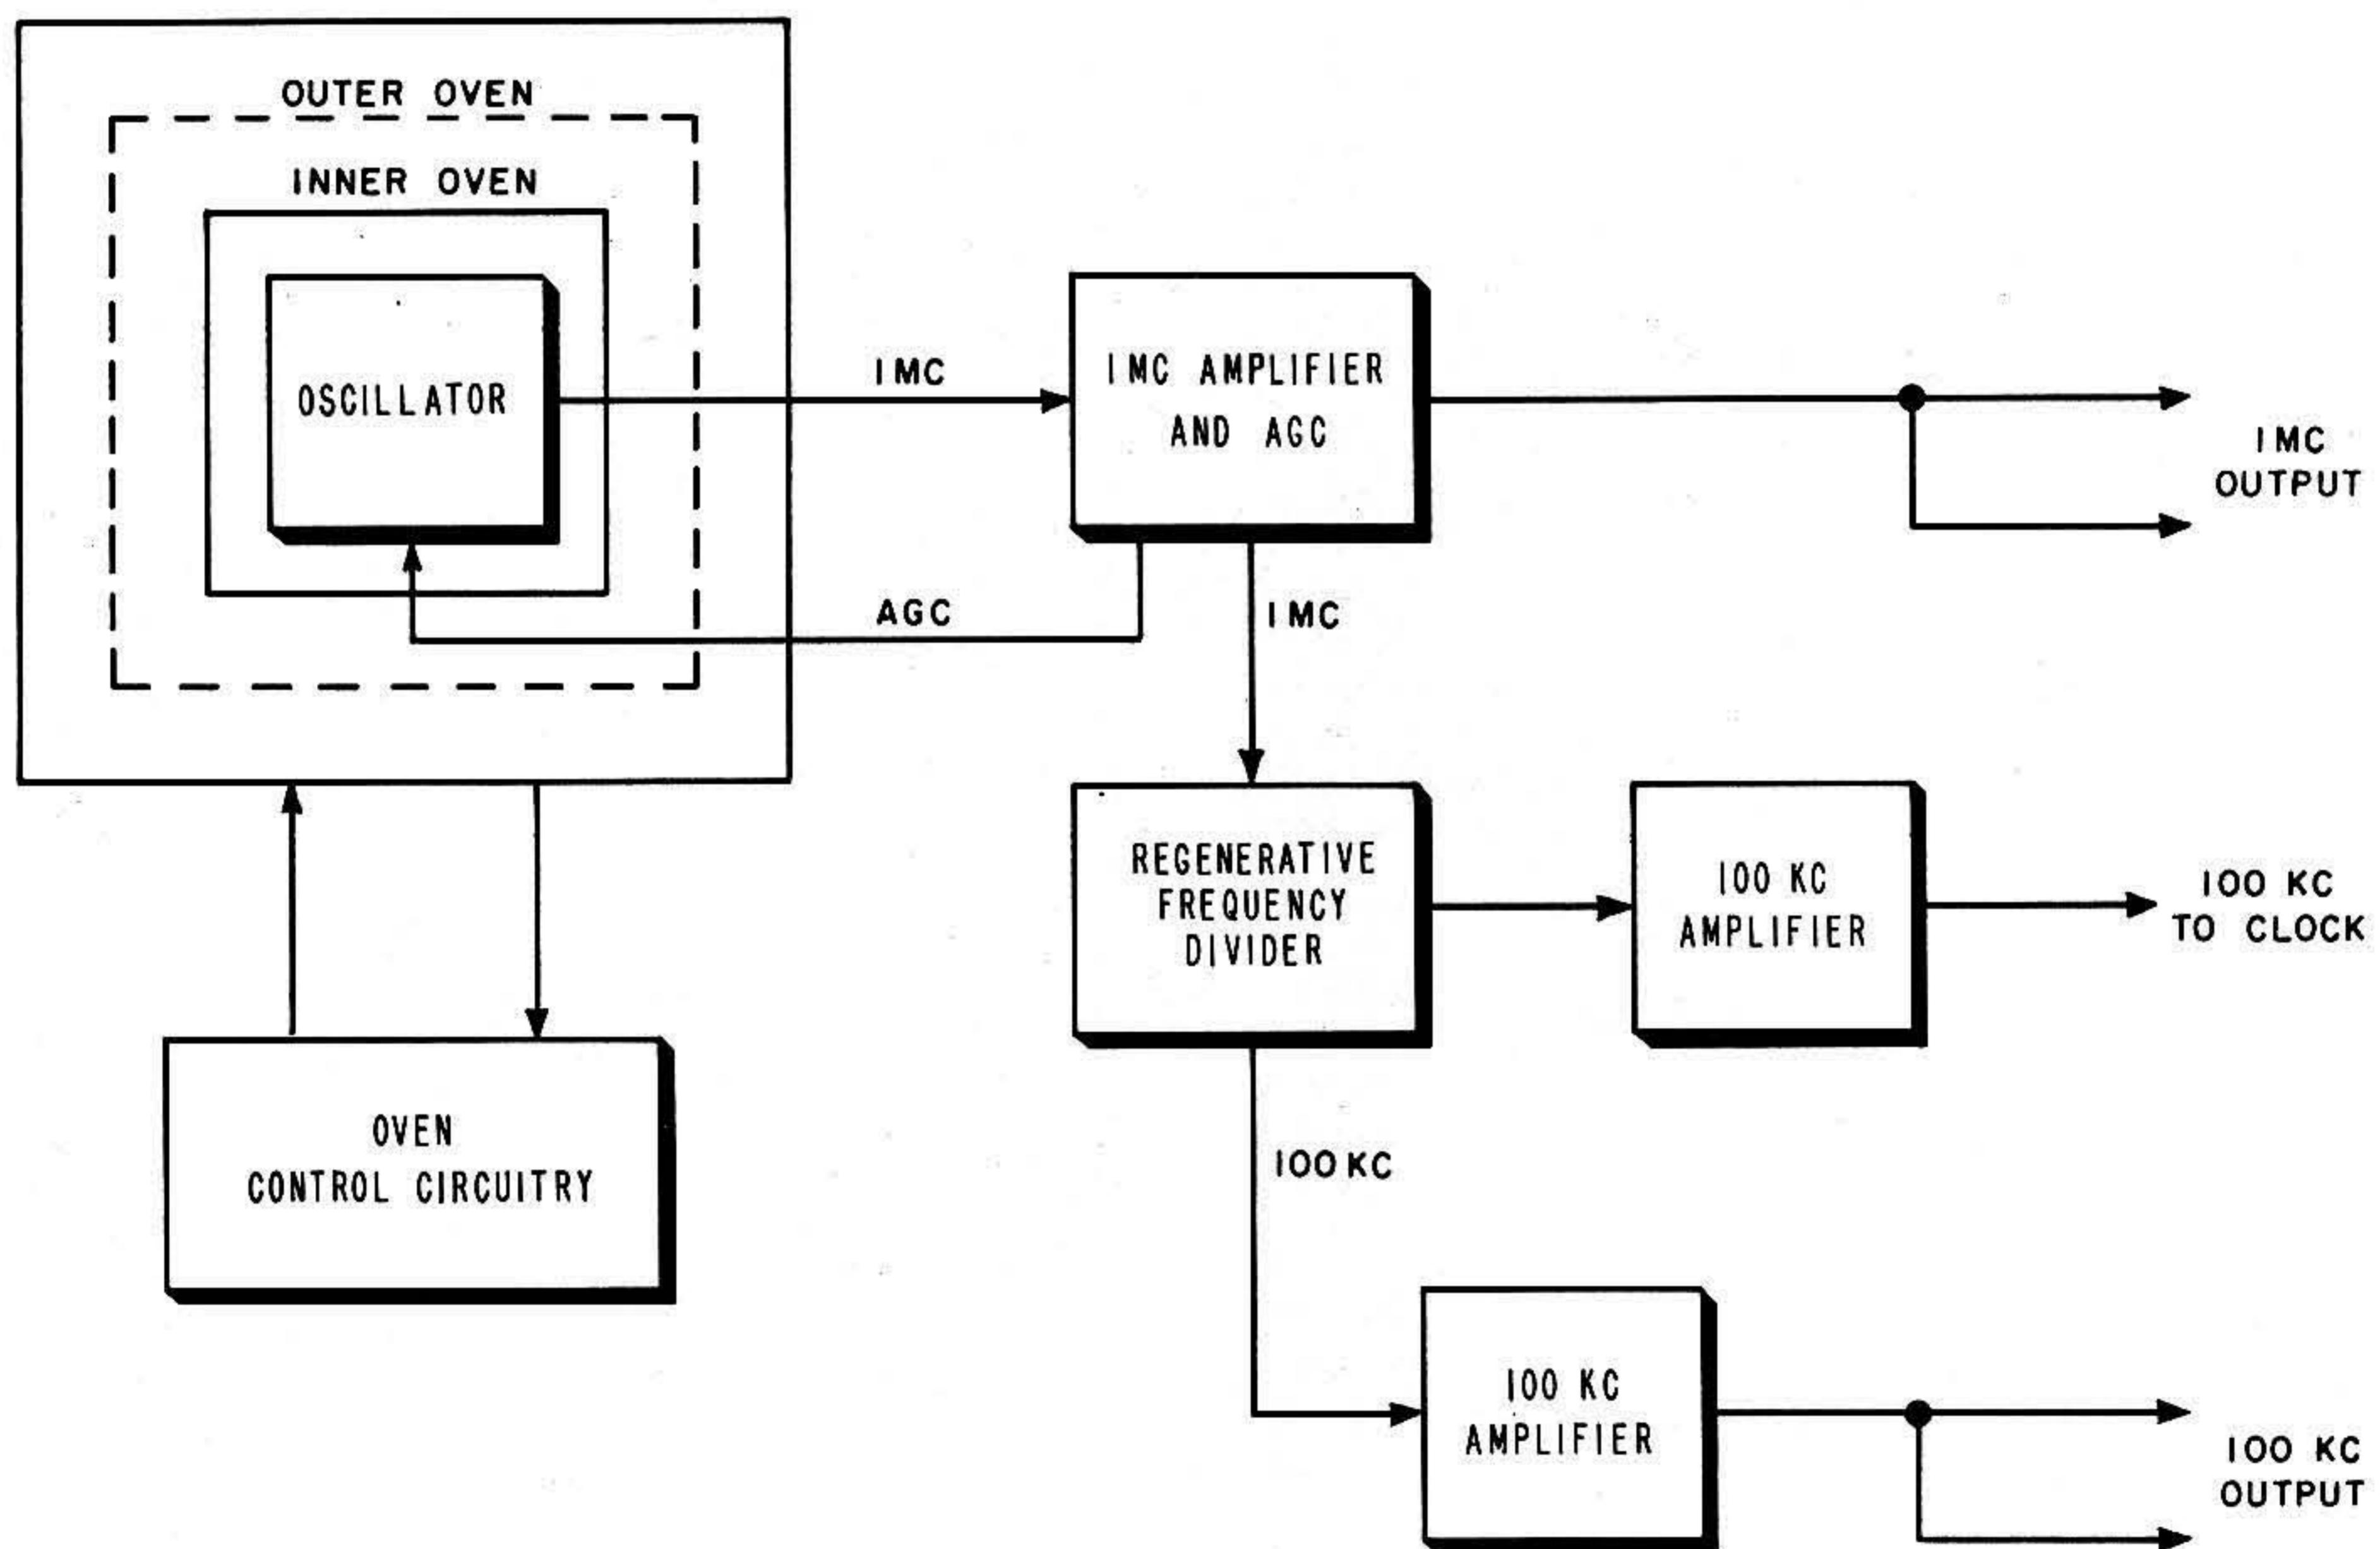


Figure 5-1. Simplified Block Diagram

SECTION IV

PERIODIC INSPECTION AND MAINTENANCE

4-1. DAILY INSPECTION.

4-2. The CIRCUIT CHECK meter indications typically are between 7.0 and 9.0 for each position of the switch. Excessive deviation from this indication indicates either marginal operation or a circuit malfunction. Keep a permanent record of CIRCUIT CHECK meter indications for maintenance purposes.

4-3. MAINTENANCE.

4-4. Little or no maintenance except daily inspection will be required for the oscillator. No lubrication is required.

SECTION V

PRINCIPLES OF OPERATION

5-1. INTRODUCTION.

5-2. Section V contains information relating to the operating theory of the oscillator. The block diagram gives an overall view and the functional diagram gives the theory of operation.

5-3. SIMPLIFIED BLOCK DIAGRAM.

5-4. Figure 5-1 is a simplified block diagram of the oscillator. The 1-mc crystal oscillator is contained in a constant temperature oven. The output of the oscillator is applied to 1-mc amplifiers and is available at two output connectors. Part of the 1-mc signal drives a regenerative frequency divider which provides a 100-kc signal. The 100 kc is amplified and supplied to output connectors.

5-5. OSCILLATOR OVEN.

5-6. The oscillator oven consists of two sections, an outer and inner oven. Both ovens operate continuously. The inner oven is 0.2 watt, the outer oven is 2 watt. When the oscillator is initially turned on, both ovens operate at maximum heat. As the oven temperature approaches the operating point, the inner and outer oven idle to low heat.

5-7. Figure 5-2 is a functional diagram of the oscillator. The oven and control circuitry consist of the following:

- a. Oven control oscillator, Q301, Q302, and T301.
- b. Detector, Q303.
- c. Temperature sensing element, RT101. Thermistor RT101 has a negative temperature coefficient. Resistors R101, RT101, and the upper two secondaries of T301 form a bridge circuit.
- d. Inner oven heater, R102, R103.

e. Inner oven heater amplifier, Q304.

f. Outer oven heater, R104, R105 (not shown on functional diagram).

g. Amplifier, Q305.

h. Outer oven heater amplifier, Q306.

5-8. Oscillation is sustained because of the regenerative feedback from the junction of R101 and RT101. The bridge approaches a balanced condition at correct oven temperature. The voltage waveforms at points A and B with respect to point C, and C with respect to ground at normal oven temperature, are shown in the waveform chart in figure 5-2. Waveform C is the resultant of A and B.

5-9. When the oven is cool, RT101 resistance is high. The bridge is very unbalanced. The voltage drop across RT101 is much larger than across R101. The voltage waveforms at points A, B, and C are now as shown in the chart at A1, B1, and C1. Waveform C1 is the resultant of the two waveforms at A1 and B1. The amplitude at C1 is now larger and causes the oven control oscillator output voltage to increase. A larger signal is applied to detector Q303 which then supplies a larger signal to the inner oven heater amplifier. This causes more current to flow through the inner oven heaters. The larger voltage drop across the inner oven heaters increases the forward bias on Q306, causing a larger outer heater current. When the oven chamber reaches its operating temperature, the bridge approaches balance and oscillator output decreases. Detector output therefore decreases, causing lower heater current.

5-10. The collector voltage of Q304 can be monitored by setting the CIRCUIT CHECK switch to INNER OVEN.

5-11. The emitter voltage of Q306 can be monitored by setting the CIRCUIT CHECK switch to OUTER OVEN.

5-12. Resistor R308 is a 23-position switch with resistance wire connected between contacts. As the switch is rotated clockwise or counterclockwise, the operating point of the oven will rise or fall. Resistor R308 changes the oven temperature approximately 0.1 degree per position. The operating point of the oven is nominally between 63 and 68 degrees centigrade.

5-13. 1 MC OSCILLATOR AND AMPLIFIERS.

5-14. Refer to the functional diagram in figure 5-2. Oscillator Q101 is a crystal controlled type. The frequency can be varied slightly by changing the capacity of the quartz crystal circuitry using the FINE and COARSE FREQ. ADJ. The FINE FREQ. ADJ. is geared to the PARTS IN 10^{10} counter. The output of the oscillator is applied to Q102, an isolation amplifier, then applied to Q103 and Q104. The collector circuit transformer of Q104 has an agc winding whose output is rectified by a voltage doubler and applied to the oscillator. The 1-mc signal is then applied to Q201 and Q202 and supplied to the output connectors. A portion of the 1-mc signal is rectified, filtered, and used in the metering circuits.

5-15. The oscillator output can be checked by setting the CIRCUIT CHECK switch to OSC. The 1-mc output can be checked by setting the CIRCUIT CHECK switch to 1 MC.

5-16. REGENERATIVE FREQUENCY DIVIDER AND 100 KC AMPLIFIERS.

5-17. The output of Q102 is also applied to Q203, amplified, and applied to a crystal mixer. Nothing further occurs until the 100 KC START button is depressed. Refer to the schematic diagram in figure 9-2. When the button is depressed, Q205, C251, L203, and C234 become a 100-kc oscillator. When the button is released, the oscillator becomes an 100-kc amplifier.

5-18. The 100-kc oscillator signal is momentarily applied to Q204, a X9 multiplier circuit. Q204 is operated in a non-linear manner to obtain harmonics in its output. One secondary of T204 is the collector load for Q204. The other secondary winding is an LC circuit resonant at 900 kc which rings upon excitation from Q204. The 900-kc signal is coupled to the primary of T204 and applied along with the 1-mc signal to the mixer. Refer to the block diagram in figure 5-2. The mixer heterodynes the two signals. Tank circuit L201 and C232 in the output of the mixer is resonant at 100 kc. The difference-frequency (100 kc) current develops a voltage across the tank circuit which is applied to Q205 and amplified.

5-19. Part of the 100-kc signal is applied to emitter follower Q206, and is available at the CLOCK output connector. Refer to figure 5-2. Part of the 100-kc signal is applied to Q207, amplified, and available at the 100 KC OUTPUT connectors.

5-20. The 100 KC OUTPUT can be monitored by setting the CIRCUIT CHECK switch to 100 KC.

5-21. POWER SUPPLY (Regulator).

5-22. The regulator uses two breakdown diodes for a voltage reference and a third as a -7 volt regulated source. Refer to the schematic, figure 8-3. The supply voltage for the regulator is between 22 and 30 volts. The output of the regulator is -20 volts regulated. Diodes CR302A and CR302B supply the base of Q307 with a -20 volt reference level. If the output voltage of the regulator becomes more negative, the forward bias on Q307 decreases. The transistor emitter-collector impedance increases, the output voltage decreases until Q307 emitter-base bias approaches 0 volt. To check the regulator output, set the CIRCUIT CHECK switch to SUPPLY.

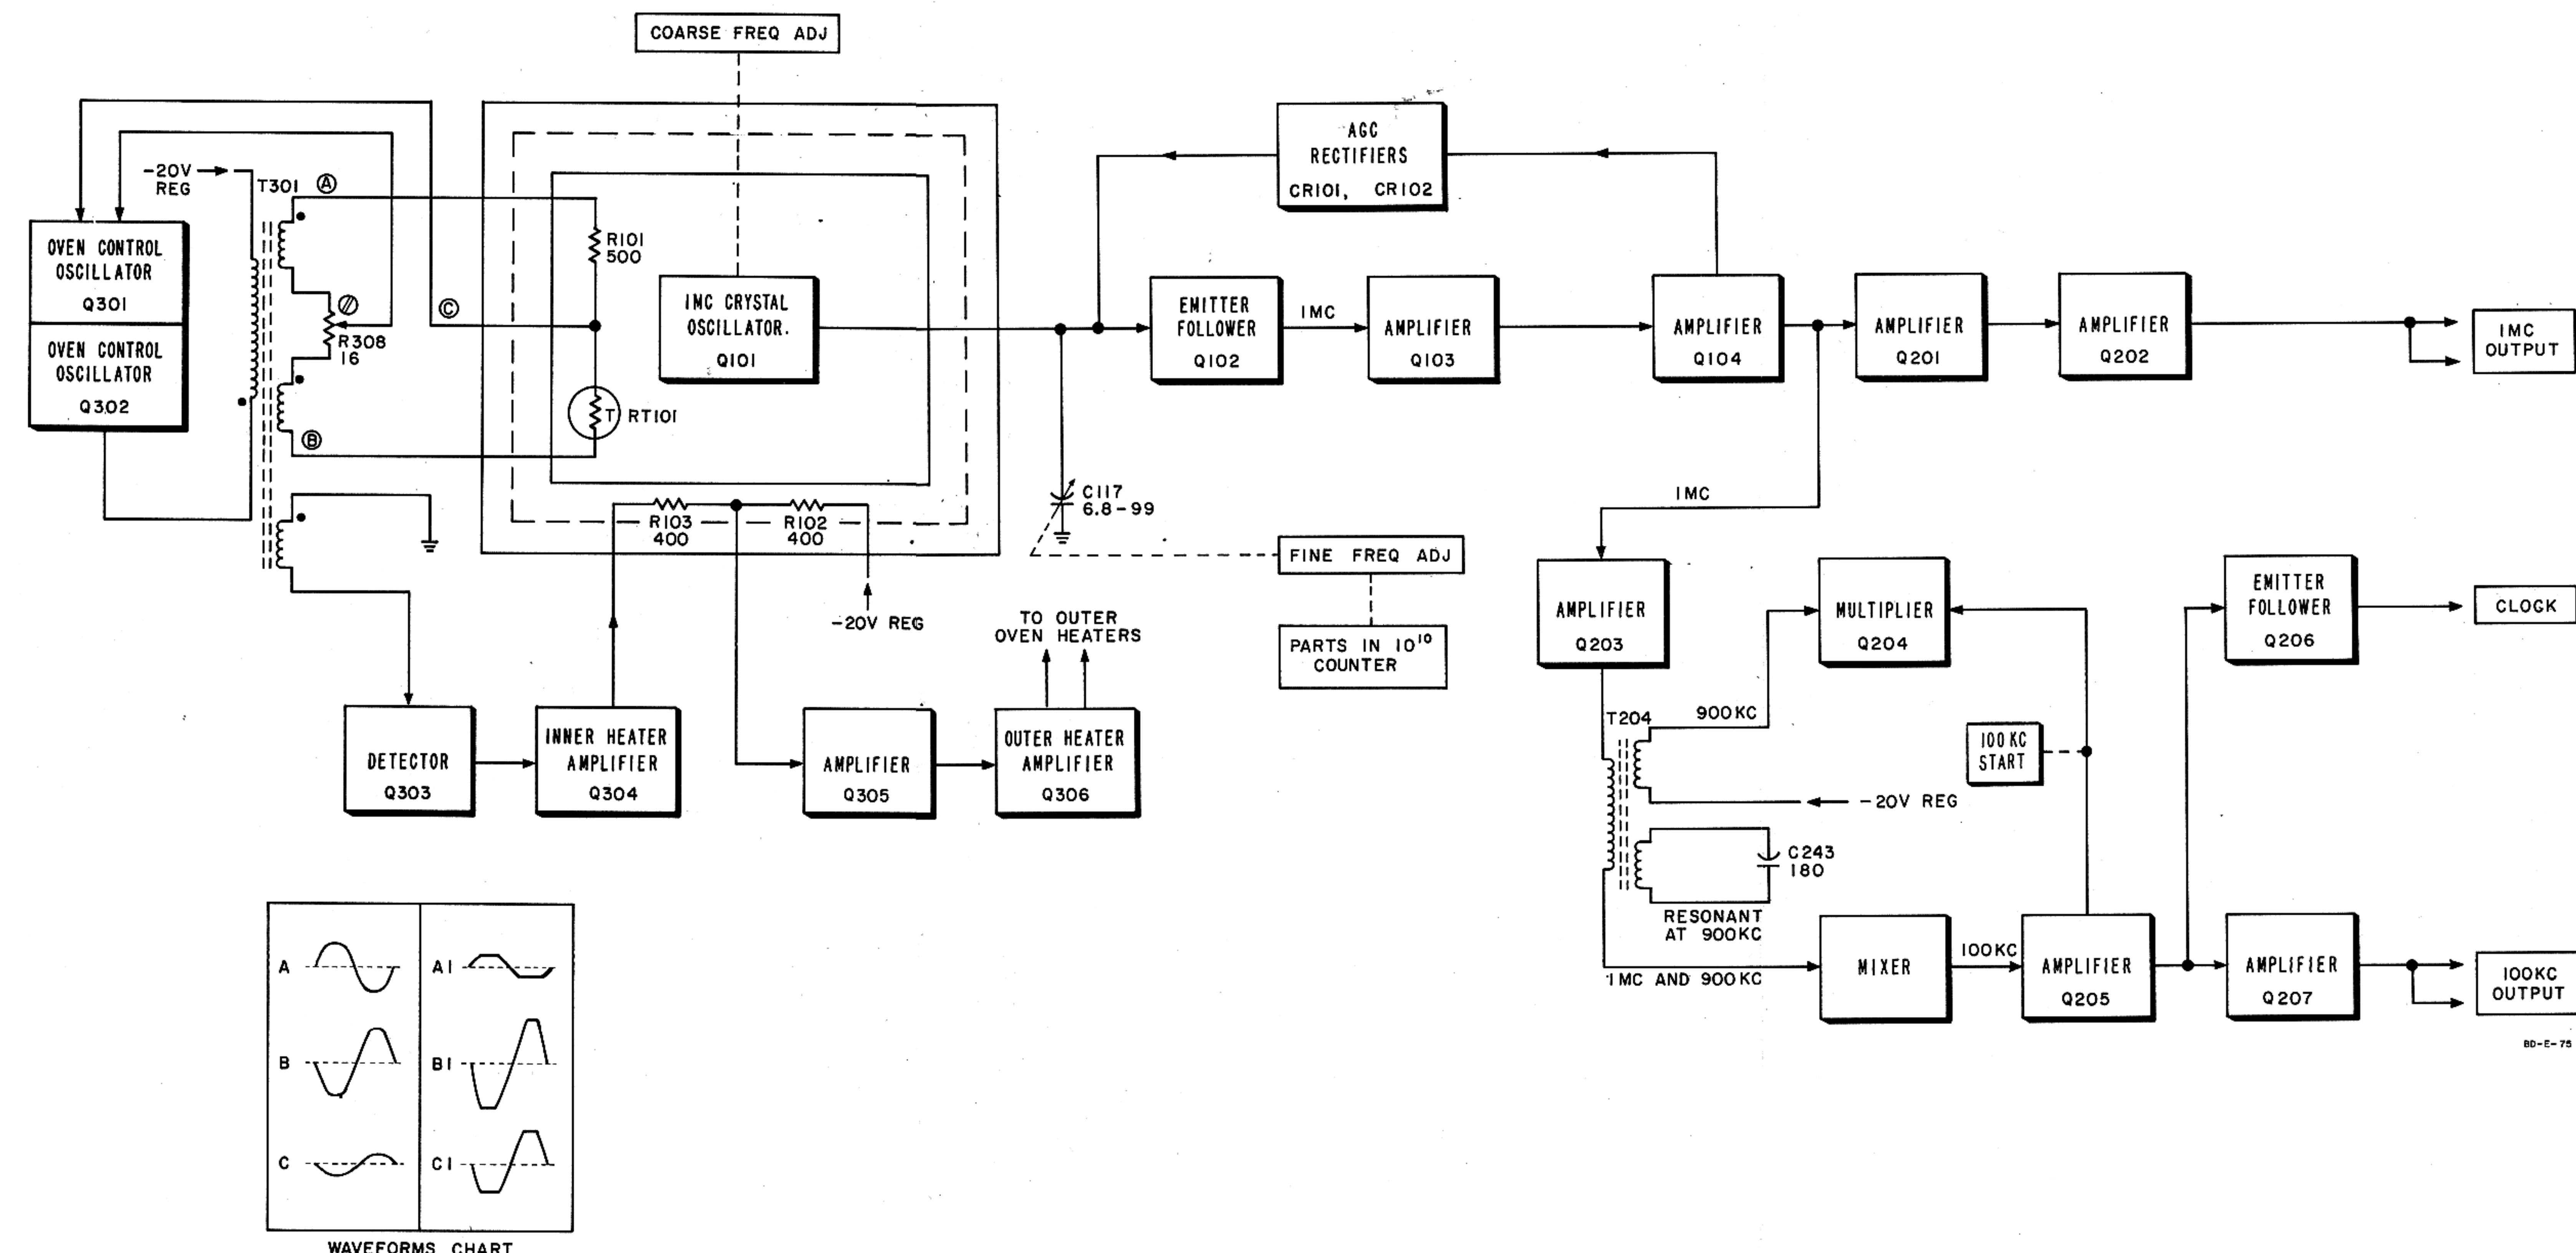


Figure 5-2. Functional Diagram

SECTION VI

TROUBLESHOOTING

6-1. GENERAL INFORMATION.

6-2. The oscillator covers can be removed for routine inspection and maintenance while in operation by removing the seven screws around the edges of top and bottom covers. Do not loosen any other screws.

6-3. The following method is recommended for finding circuit failures:

a. Sectionalization. Sectionalize trouble by evaluating front-panel symptoms. See paragraph 6-6.

b. Localization. Localize trouble by making voltage checks in the defective section. See paragraph 6-9.

c. Substitution. Check for failure of individual components by substitution, resistance measurements, etc.

6-4. TEST EQUIPMENT.

6-5. The following test equipment or its equivalent is required for troubleshooting the oscillator:

a. Oscilloscope: Frequency range, dc to 1 mc, such as Φ Model 150A.

b. DC Vacuum Tube Voltmeter: Voltage range 0.1 to 30 volts, such as Φ Model 412A.

c. AC Vacuum Tube Voltmeter: Frequency range 100 kc to 1 mc, such as Φ Model 400D.

d. Signal Generator: Frequency range 100 kc to 1 mc, such as Φ Model 650A.

6-6. SECTIONALIZATION.

6-7. To determine the general location of a faulty circuit, proceed as follows. Set the CIRCUIT CHECK switch to each position and note the meter indication. If a particular meter indication is not within the limits listed in table 6-1, troubleshoot the circuit to which the CIRCUIT CHECK switch is positioned.

6-8. If the CIRCUIT CHECK meter indicates all circuits except the 100-kc circuits are normal, and the 100-kc meter indication is "0", try restarting the regenerative frequency divider. Momentary power or signal interruption may have stopped the divider. See paragraph 2-12 to start the divider. If the regenerative divider will not start and 1-mc meter indication is normal, troubleshoot the regenerative divider circuits.

6-9. LOCALIZATION.

6-10. After determining which section of the oscillator is defective, make dc voltage checks on the emitter, base, and collector of the transistors involved. Typical dc voltages for each stage are shown on the schematics. The voltages in parentheses are measured with the regenerative frequency divider non-operating.

Table 6-1. Circuit Check Meter Indications

CIRCUIT CHECK Switch Position	Meter Indication
SUPPLY	7.0 to 9.0
OSC	7.0 to 9.0
INNER OVEN	7.0 to 9.0
OUTER OVEN (cold)	full scale
OUTER OVEN (warm)	7.0 to 9.0 (at ambient temperature of 25°C)
1 MC	7.0 to 9.0
100 KC	7.0 to 9.0

Note: The 1 MC and 100 KC meter indications may be lower than above if outputs are connected to load

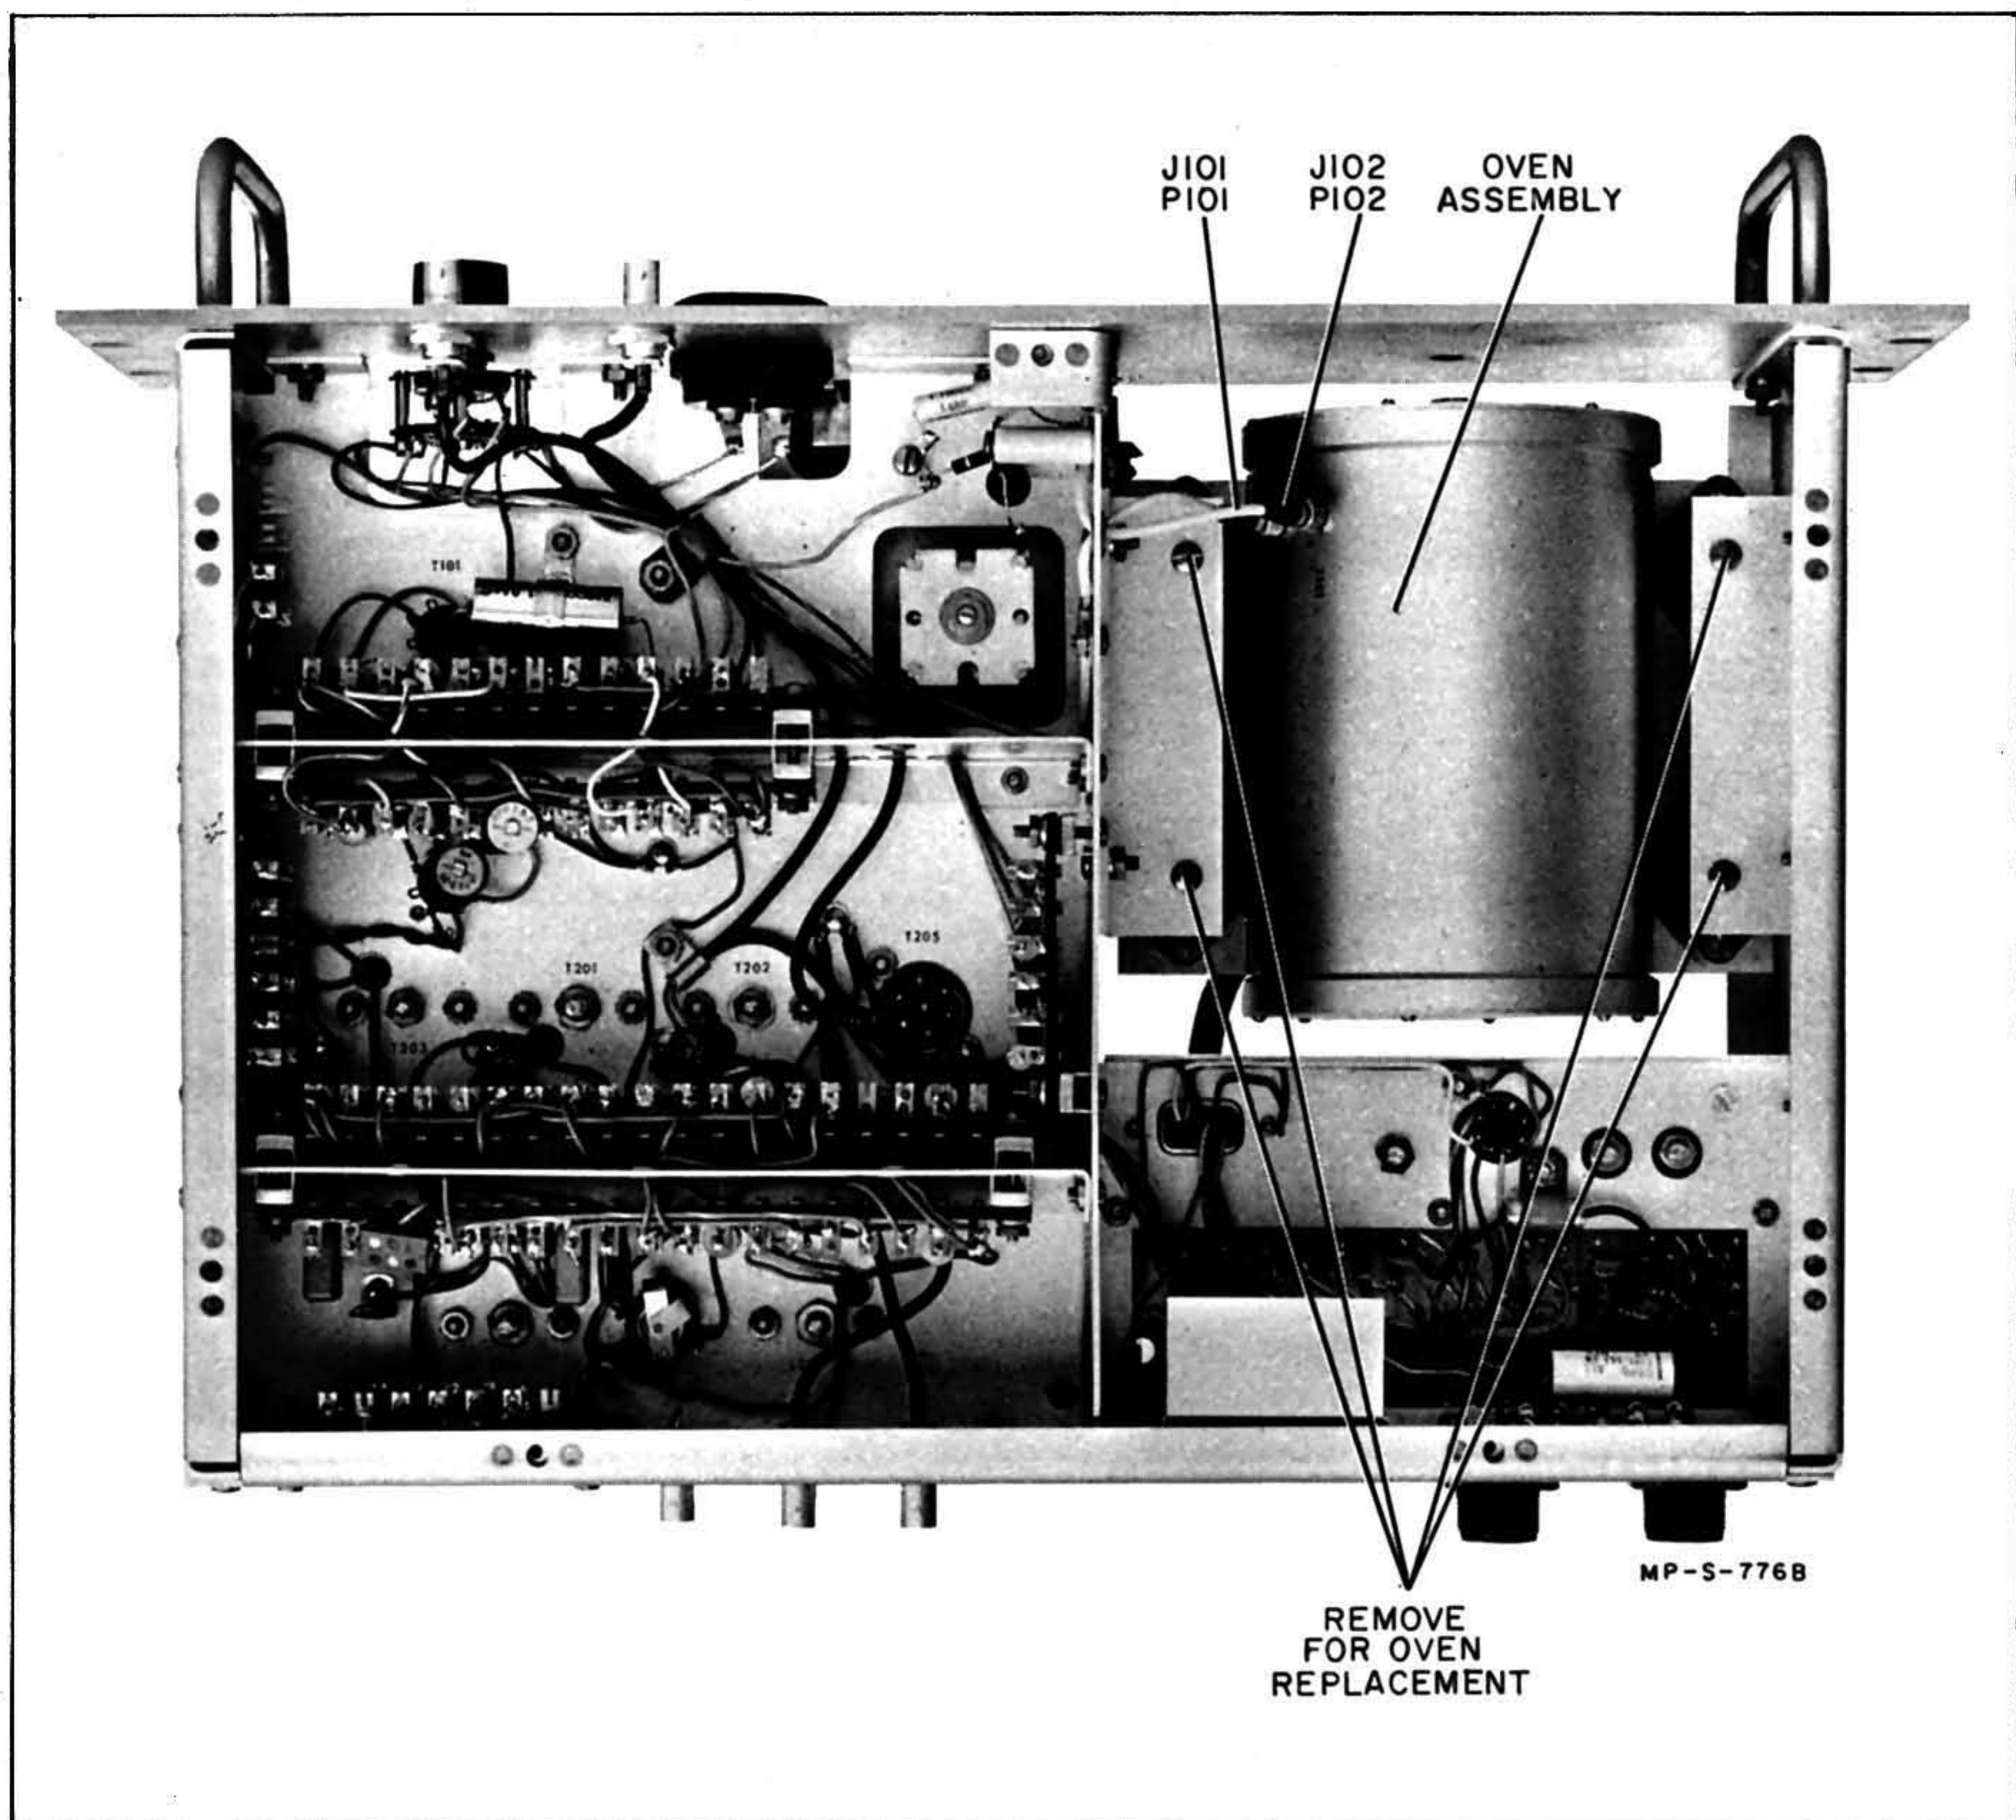


Figure 7-1. Bottom View Model 103AR

SECTION VII

REPAIRS

7-1. SECTIONS REQUIRING SPECIAL ATTENTION.

7-2. OSCILLATOR OVEN.

7-3. If it is determined the malfunction is located in the oven, DO NOT DISMANTLE the oven. It is a semi-sealed unit and must be sent to the factory for repairs. Guarantee is voided if oven is tampered with. To remove the oven, proceed as follows:

- a. Remove power from the oscillator.
- b. Disconnect P103 from J103, P101 from J101, and P102 from J102. See figures 7-1 and 7-2.
- c. Remove the screw in the shock mount at each corner of the oven. See figure 7-1.

d. Carefully remove the oven from the frequency standard. Pack and prepare oven for shipment. See paragraph 2-3.

7-4. When the oven is returned from the factory and installed in the oscillator, connect the oscillator to power. If necessary adjust oven operating point. See paragraph 8-11 to set operating point.

7-5. TRANSISTORS Q102, Q103, and COMPONENTS.

7-6. Before any repairs are made on Q102 or Q103 circuits, disconnect P101 and P102 from the oven. This action prevents crystal damage.

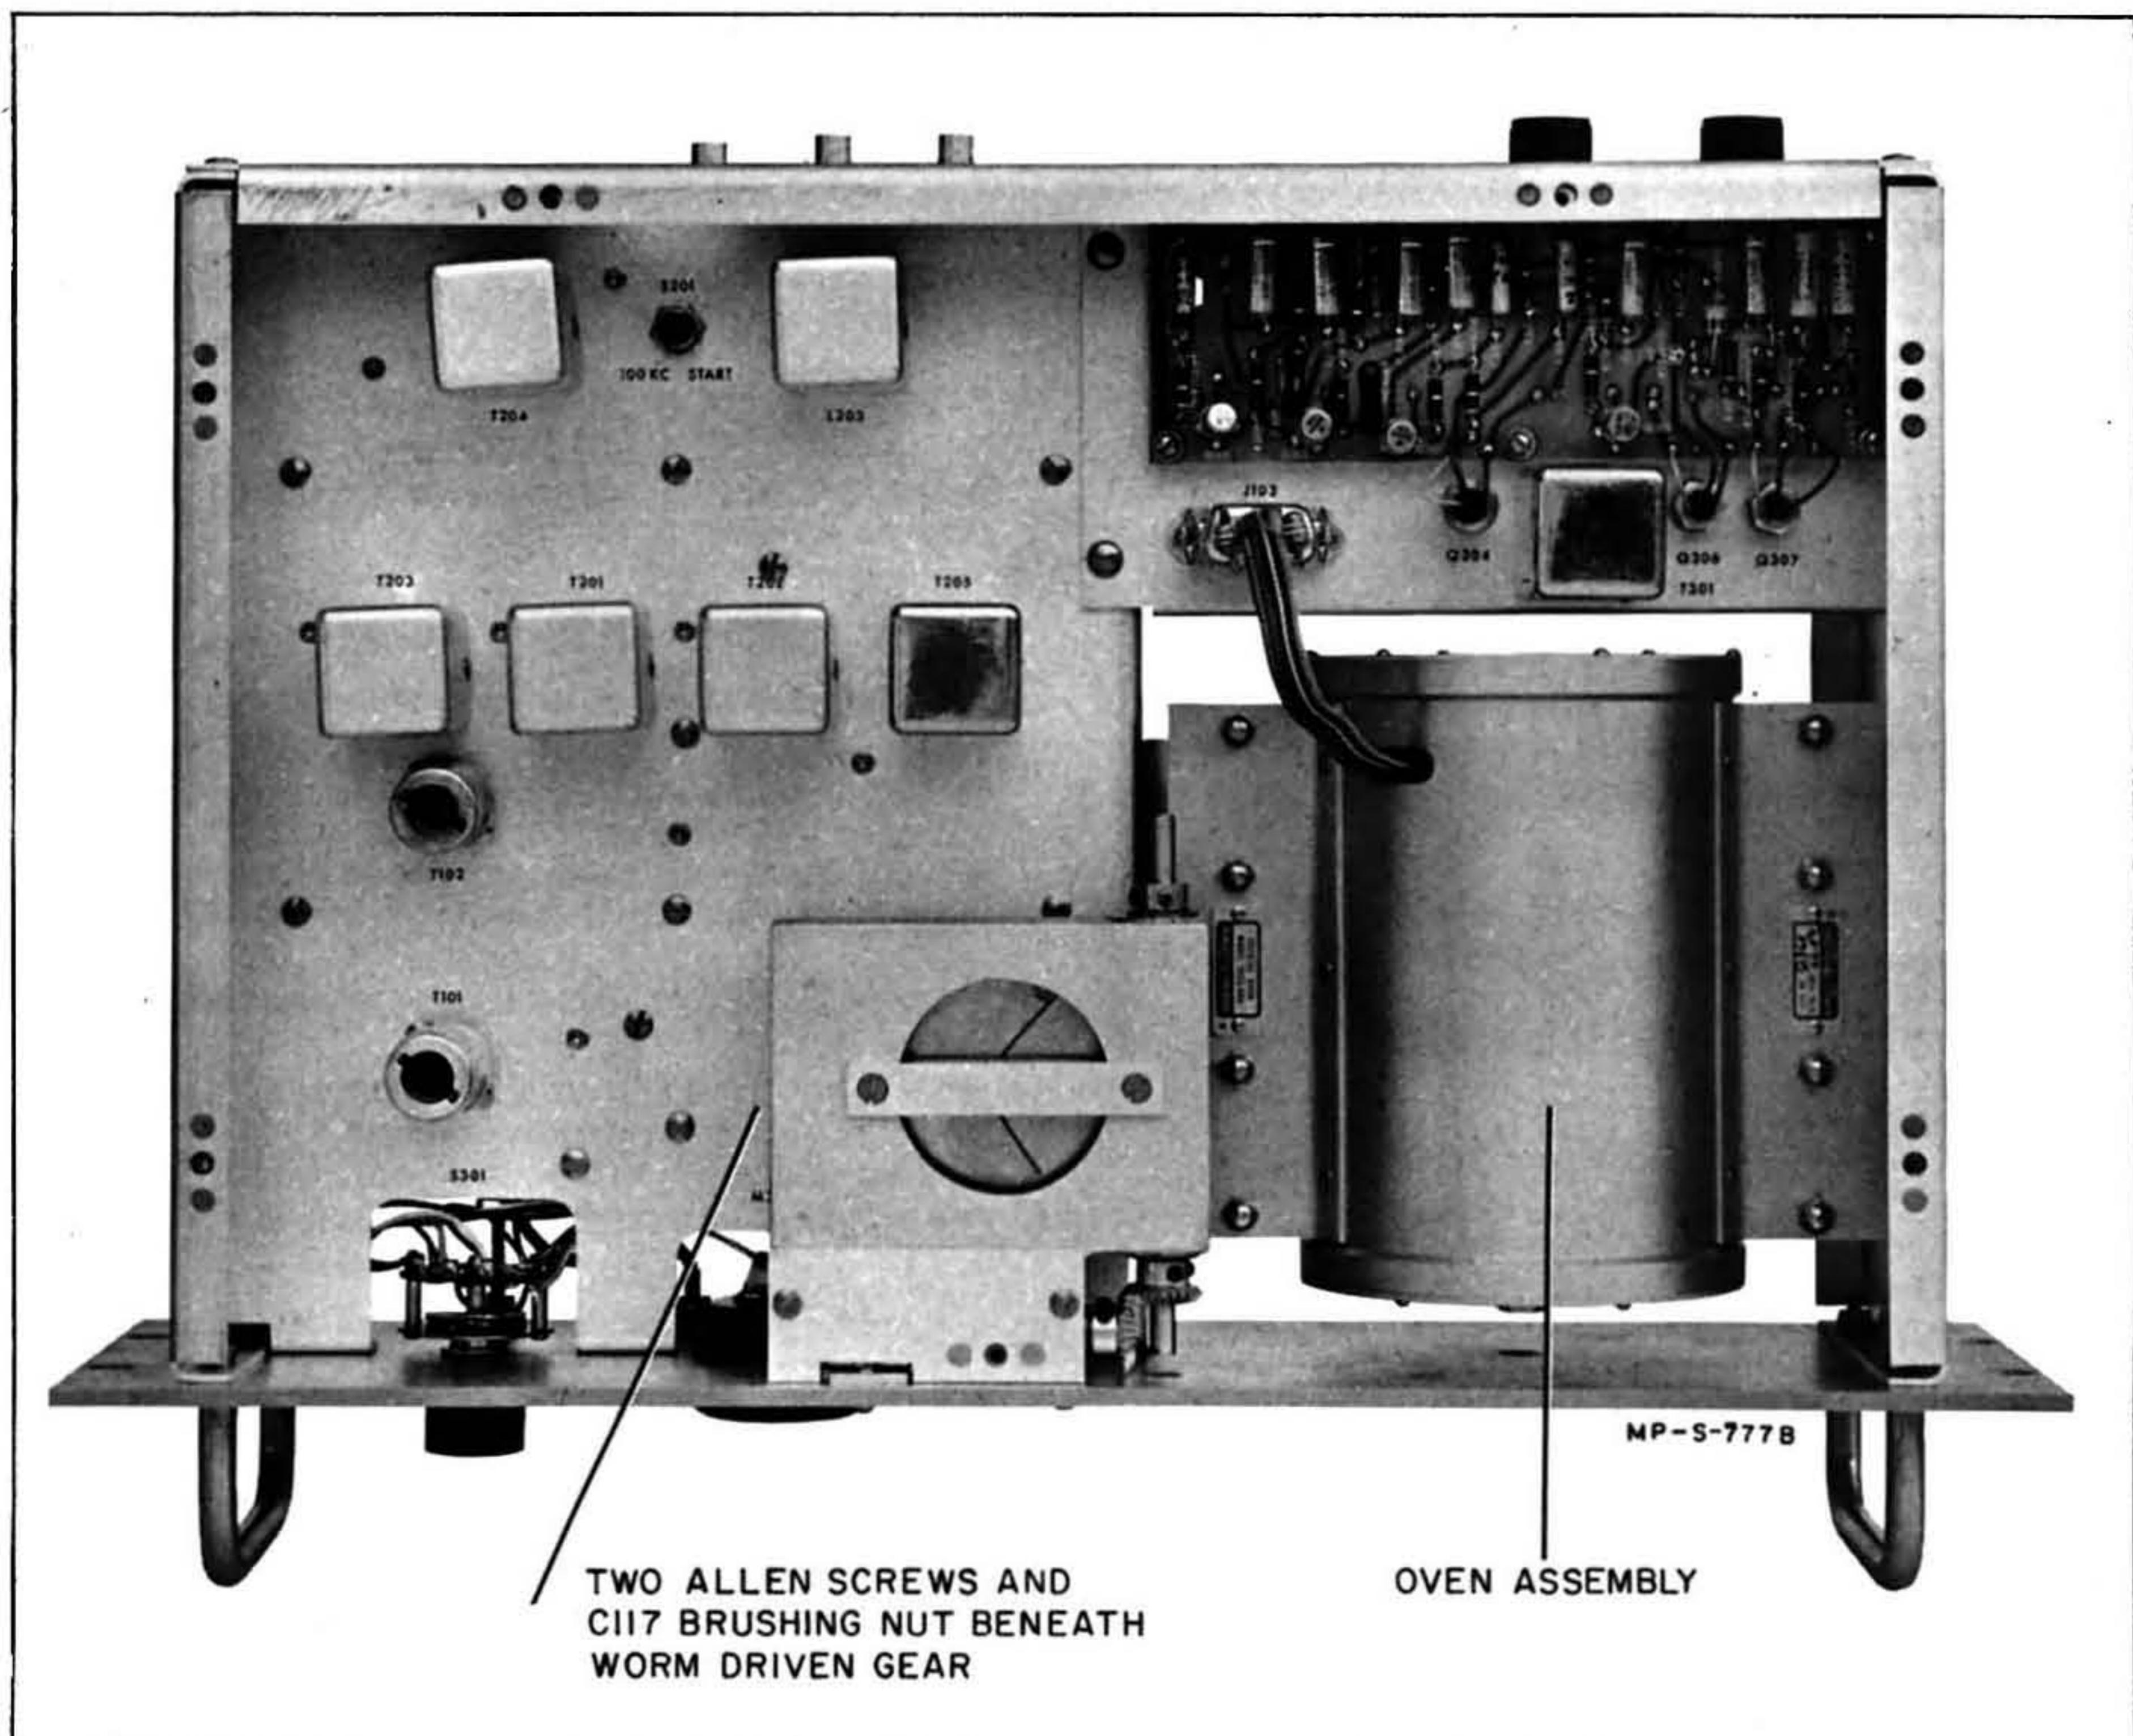


Figure 7-2. Top View Model 103AR

7-7. TRANSISTORS Q201, Q202, Q205, Q207, and COMPONENTS.

7-8. When components in Q201 or Q202 circuits are replaced, check the 1 MC OUTPUT. The output voltage should be between 1.0 and 1.1 volts with a 50-ohm load connected to the 1 MC OUTPUT. If necessary change R220 to obtain 1.0 to 1.1 volts. Then connect an oscilloscope such as the Φ Model 150A to the emitter of Q202. The waveform should be a sine wave with little or no clipping or distortion.

7-9. When components in Q205 or Q207 are replaced, check the 100 KC OUTPUT. The output voltage should be between 1.0 and 1.1 volts with a 50-ohm load connected to the 100 KC OUTPUT. If necessary, change R280 to obtain 1.0 to 1.1 volts. Then connect an oscilloscope such as the Φ Model 150A to the emitter of Q207. The waveform should be a sine wave with little or no clipping or distortion.

7-10. TRANSISTORS Q102, Q103, Q104, and COMPONENTS.

7-11. Before components in Q102, Q103, or Q104 circuits are replaced disconnect P101 and P102 from the oven. This action will prevent damage to the crystal.

7-12. TRANSISTOR AND COMPONENTS REPLACEMENT.

7-13. Power to the oscillator must be removed only when repairs to the oven control or power supply regulator circuits are being made. When making repairs to other circuits, power to the oscillator should not be removed. The wire supplying the collector voltage to the circuit under repair should be disconnected. After repairs are completed, the wire must be reconnected.

7-14. When transistors are soldered in the circuits, care must be used so transistors do not become overheated.

7-15. When replacing power transistors be careful so the mica insulating disc is not broken or cracked.

7-16. OUTPUT SIGNAL LOADING.

7-17. When the signal output voltages are being checked or adjusted, a 50-ohm load must be connected to the appropriate output connector.

7-18. CAPACITOR C117 REPLACEMENT.

7-19. To replace C117 disconnect P101 and P102 from oven before removing defective C117. Then note C117 rotor position. Set the replacement capacitor rotor to the same position as rotor of defective capacitor. This may prevent the oscillator error from being excessive. To remove C117 proceed as follows:

- a. Unsolder and remove wires from C117.
- b. Loosen the two allen screws on the worm driven gear. See figure 7-2.
- c. Using a 3/8 inch flat open end wrench, remove the nut on the front bushing of C117.
- d. Remove C117; then install new capacitor.
- e. Replace and tighten nut on bushing. Tighten the two allen screws. Be sure the worm driven gear turns easily.
- f. Replace and resolder wires to C117.
- g. Reconnect P101 and P102.
- h. Check frequency. If necessary adjust C117. See paragraph 3-10.

7-20. RESISTOR R308 REPLACEMENT.

7-21. If it becomes necessary to replace R308, proceed as follows:

- a. Note the rotor position of R308.
- b. Set the rotor of the replacement resistor to the same position as defective R308. Replace the defective resistor.
- c. Apply power to the oscillator. Check the oscillator stability after several days operation.

If the stability has changed, adjust oven control R308. See paragraph 8-11.

SECTION VIII

TESTING AND ADJUSTMENT

8-1. PERFORMANCE CHECK.

8-2. If the oscillator appears to be operating properly, as indicated by correct output signals and CIRCUIT CHECK meter indications, all basic circuits in the oscillator are operating properly.

8-3. CIRCUITS REQUIRING ADJUSTMENT.

8-4. When certain components are replaced, adjustments may be necessary. Table 8-1 lists the components and circuits that may need adjustment.

8-5. ADJUSTMENTS.

8-6. AMPLIFIER Q103 and Q104 NEUTRALIZATION.

a. Connect an ac meter such as the \oplus Model 400D to the 1 MC OUTPUT connector. Disconnect P101 and P102 from J101 and J102.

b. Disconnect R129, a 2900-ohm resistor from the junction of R125 and R126. Connect loose end of R129 to same ground point to which R126 is connected.

c. Install a short across the secondary of T101. Be careful; make certain the short does not include C123.

d. Short the center conductor of P102 to ground at the point where R126 is grounded.

e. Using a signal generator such as the \oplus Model 650 Test Oscillator, apply a 1-mc $\pm 5\%$ signal to the collector of Q104 through a 150,000 ohm isolation resistor. Adjust C125 for maximum indication on the meter.

f. Remove the short from T101.

g. Adjust the signal generator above and below 1 mc. If maximum indication does not occur at 1 mc, set the signal generator to 1 mc. If maximum indication occurs at 1 mc, omit steps h and i.

h. If maximum indication in step g did not occur at 1 mc, adjust C126 until maximum indication on the meter occurs at 1 mc.

i. Repeat steps e through h.

j. Reconnect R129 to C124.

k. Disconnect the signal generator from the frequency standard.

m. Reconnect P101 and P102 to J101 and J102.

8-7. TUNED AMPLIFIER Q201.

a. Connect an ac meter such as the \oplus Model 400D to the 1 MC OUTPUT.

b. Adjust T201 for maximum meter indication.

8-8. TUNED AMPLIFIER Q202.

a. Connect an ac meter such as the \oplus Model 400D to the 1 MC OUTPUT.

b. Adjust T202 for maximum meter indication.

8-9. TUNED AMPLIFIER Q203.

a. Connect an ac voltmeter such as the \oplus Model 400D to the 100 KC OUTPUT.

b. Start the regenerative divider.

c. Adjust T203 for maximum indication on the meter.

8-10. REGENERATIVE DIVIDER Q204, Q205.

a. Connect a signal generator such as the \oplus Model 650A across tank circuit L201, C232. Apply a 100 kc $\pm 5\%$ signal to the tank circuit.

b. Connect an ac meter such as the \oplus Model 400D to the 100 KC OUTPUT connector.

c. Adjust L203 for maximum indication on the meter.

d. Disconnect the signal generator from the oscillator. Depress the 100 KC START button and adjust T204 for maximum indication on the meter.

e. Release the 100 KC START button. The regenerative divider should operate. If the divider fails to operate, repeat steps c and d.

f. Readjust L203 and T204 for maximum output.

8-11. OVEN CONTROL ADJUSTMENT.

a. Connect the 1-mc output of the oscillator to the vertical input of an oscilloscope such as an \oplus Model 150A with 152B Dual Channel Amplifier.

b. Connect the 1-mc output of a frequency standard of equal or better accuracy than the oscillator to the horizontal input of the oscilloscope.

c. Observe the presentation on the crt for a zero beat, identified by a stationary pattern.

d. Adjust the oscillator FINE FREQ. ADJ. for a stationary pattern (if not stationary in step c). Record the change of PARTS IN 10¹⁰ counter.

e. Adjust R308 one position, either way. Wait 45 minutes, to allow the oven temperature to stabilize.

f. Turn the FINE FREQ. ADJ. until a zero beat is observed on the oscilloscope. Record the change of PARTS IN 10^{10} counter.

g. Adjust R308 one position in the same direction as in step e.

h. After 45 minutes obtain a zero beat on the oscilloscope by adjusting the oscillator FINE FREQ. ADJ. Record the change on PARTS IN 10^{10} counter. If the change in parts in 10^{10} is becoming smaller, repeat steps f and g until a very small change in parts in 10^{10} is noted. The oscillator crystal operating point is then at the vertex of the curve in figure 8-1.

i. Repeat steps f and g four more times. The change in parts in 10^{10} should become larger. Plot the curve as shown in the sample curve of figure 8-1.

j. If the change in parts in 10^{10} in step h has been becoming larger instead of smaller, return R308 to its original position. Then adjust R308 one position

in a direction opposite that in step e and note the change in parts in 10^{10} . The change in parts in 10^{10} should become smaller for each position R308 is changed.

k. Repeat steps f through j.

m. When a curve similar to figure 8-1 is obtained, adjust R308 back the number of positions necessary to place the crystal operating point at the vertex of the curve. For example, if from 328 to 340 parts in 10^{10} in figure 8-1, R308 was changed three times, then back R308 three positions. The crystal operating point will then be at the vertex of the curve.

Table 8-1. Circuits Requiring Adjustment

Area of Repair	Adjustment Required	Paragraph Reference
Q103,Q104	C125,C126	7-6, 8-5
Q201	T201	7-7, 8-7
Q202	T202	7-7, 8-9
Q203	T203	8-11
Q204,Q205	L203,T204	8-10

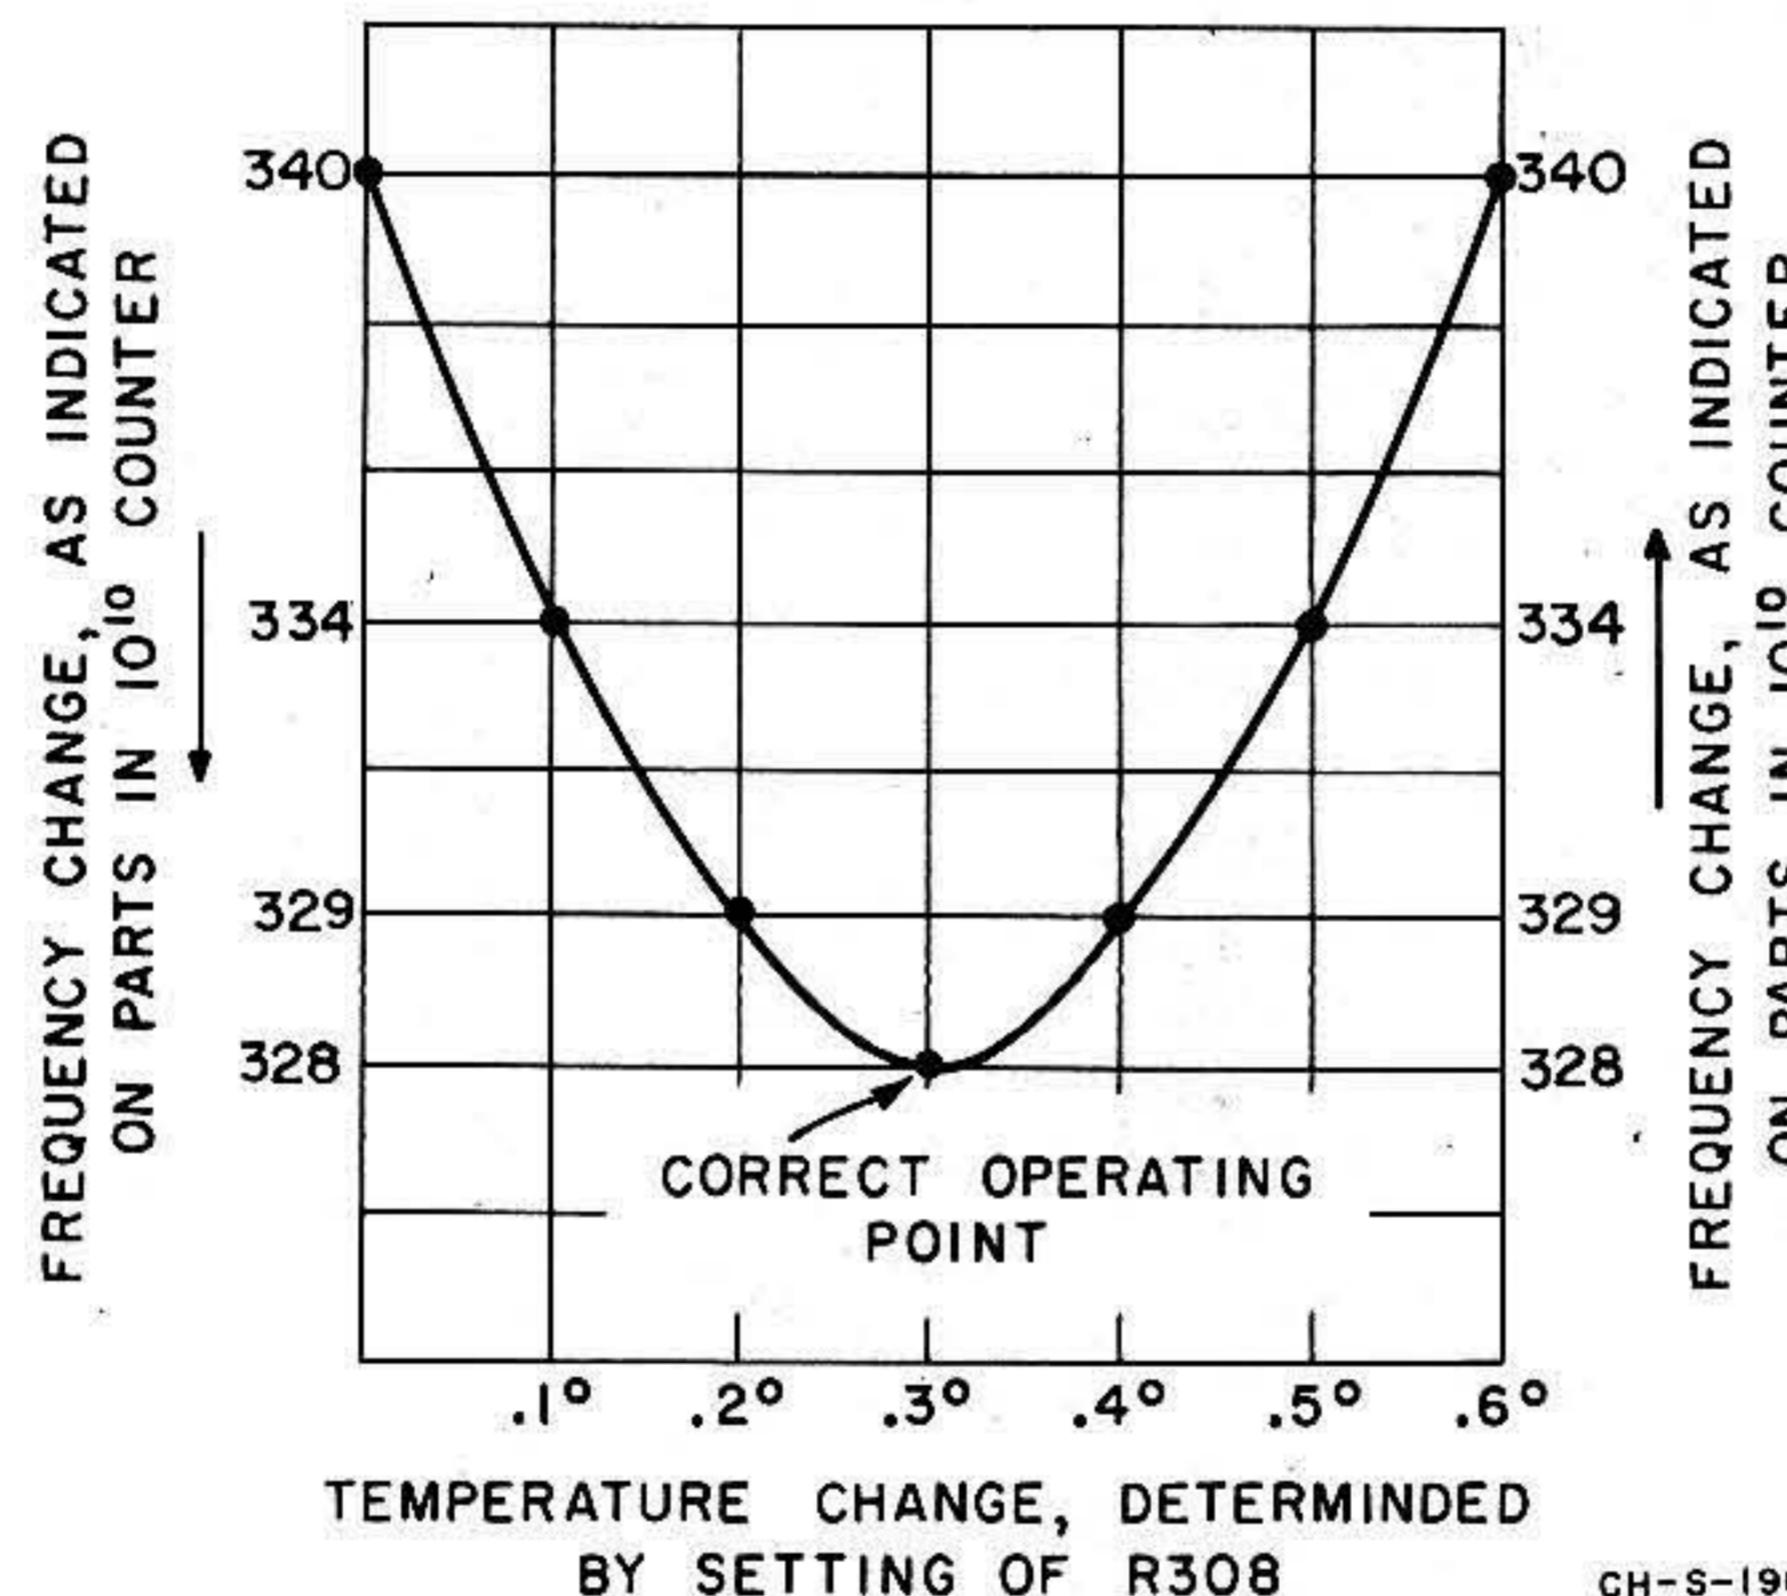


Figure 8-1. Sample Curve

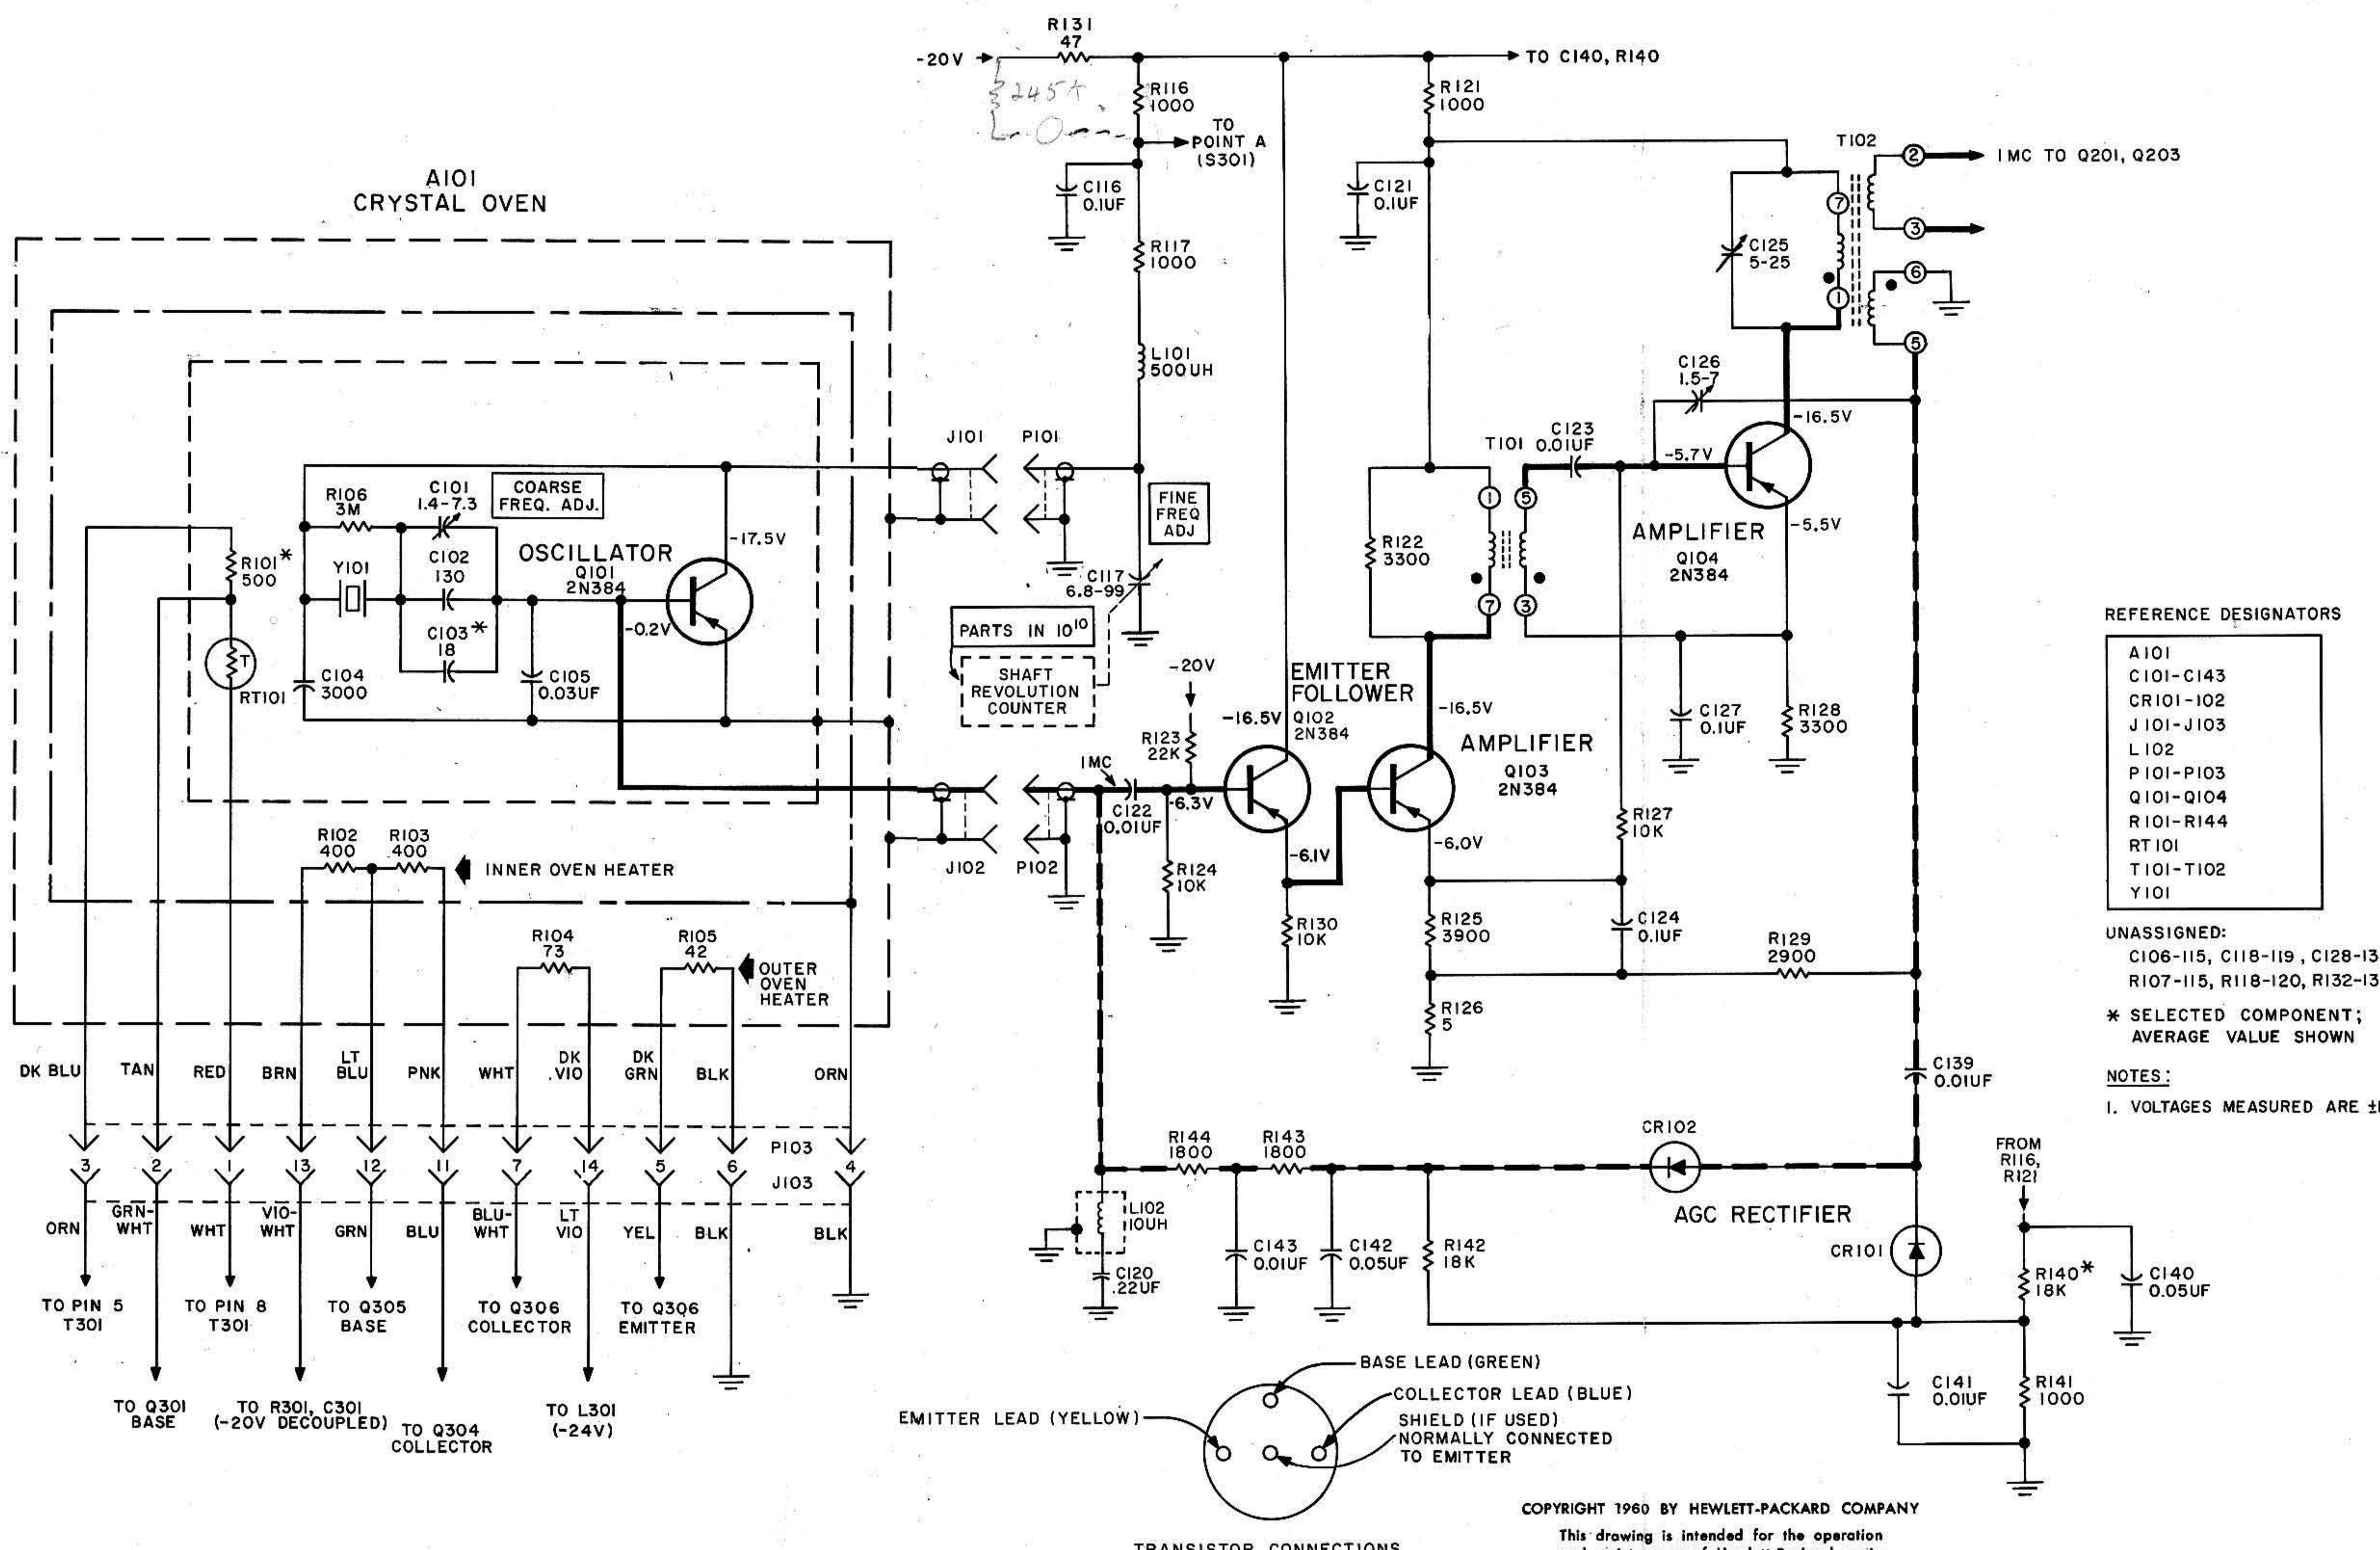


Figure 8-2. Oscillator

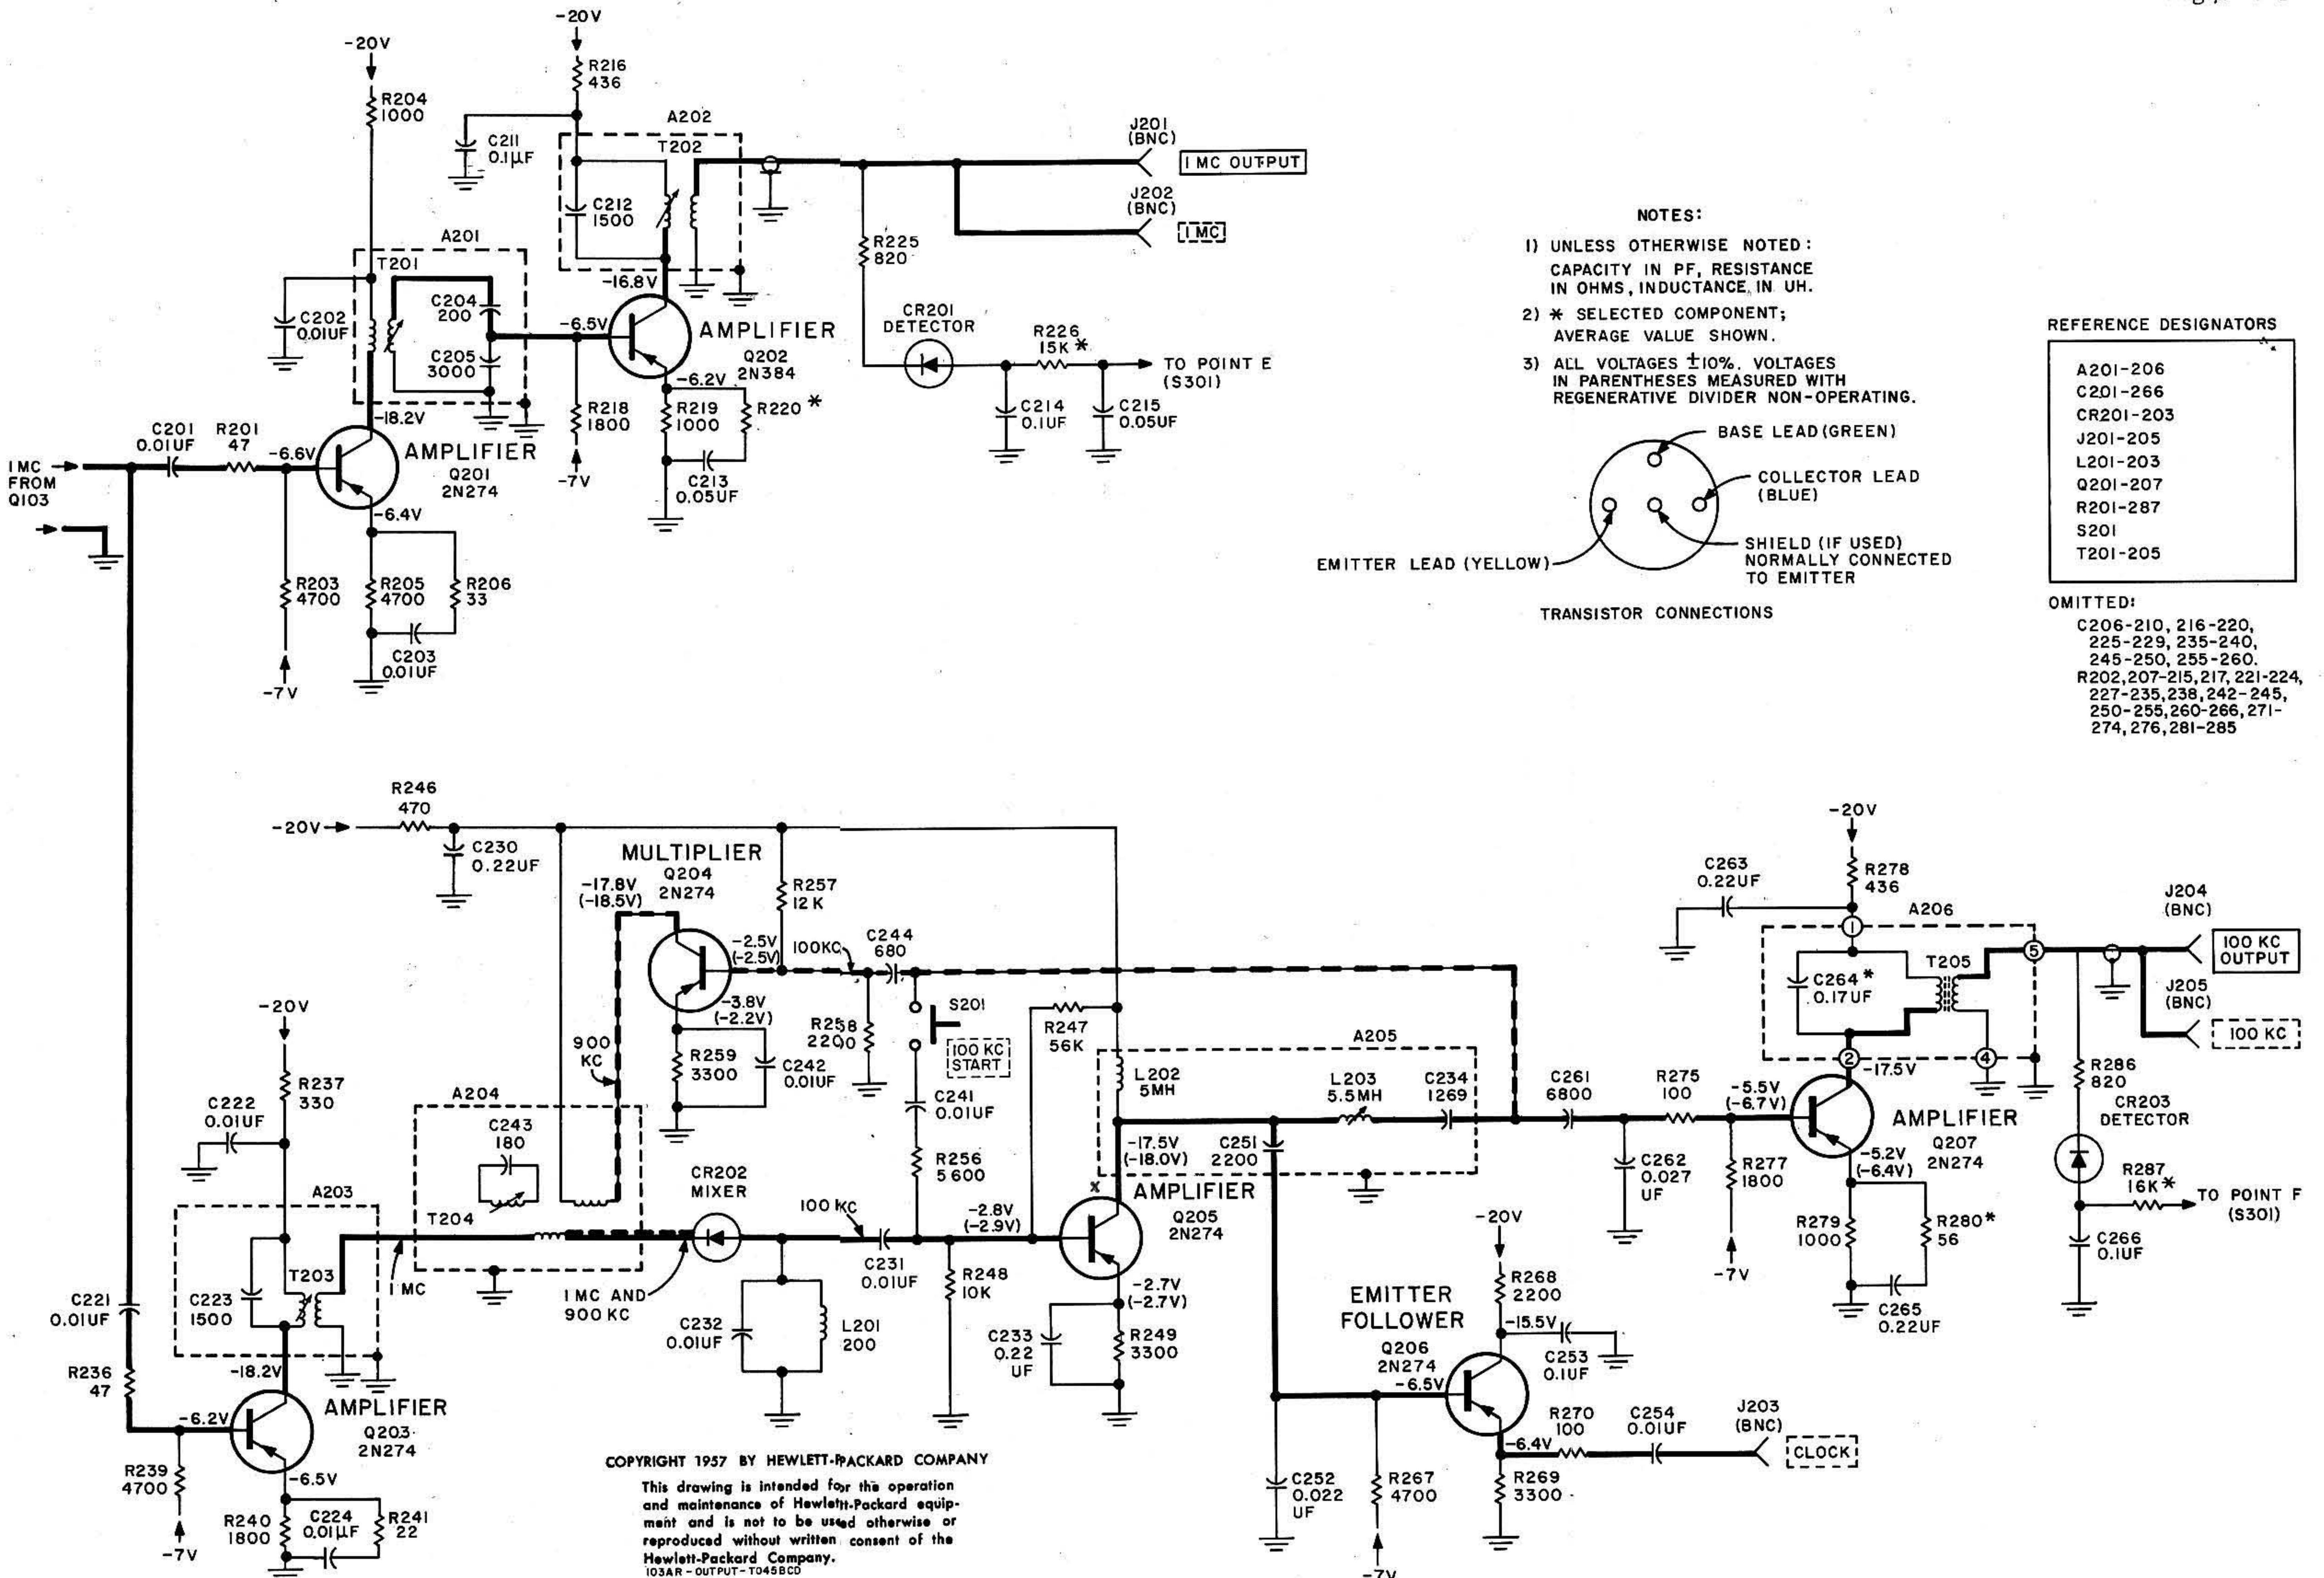


Figure 8-3. Output

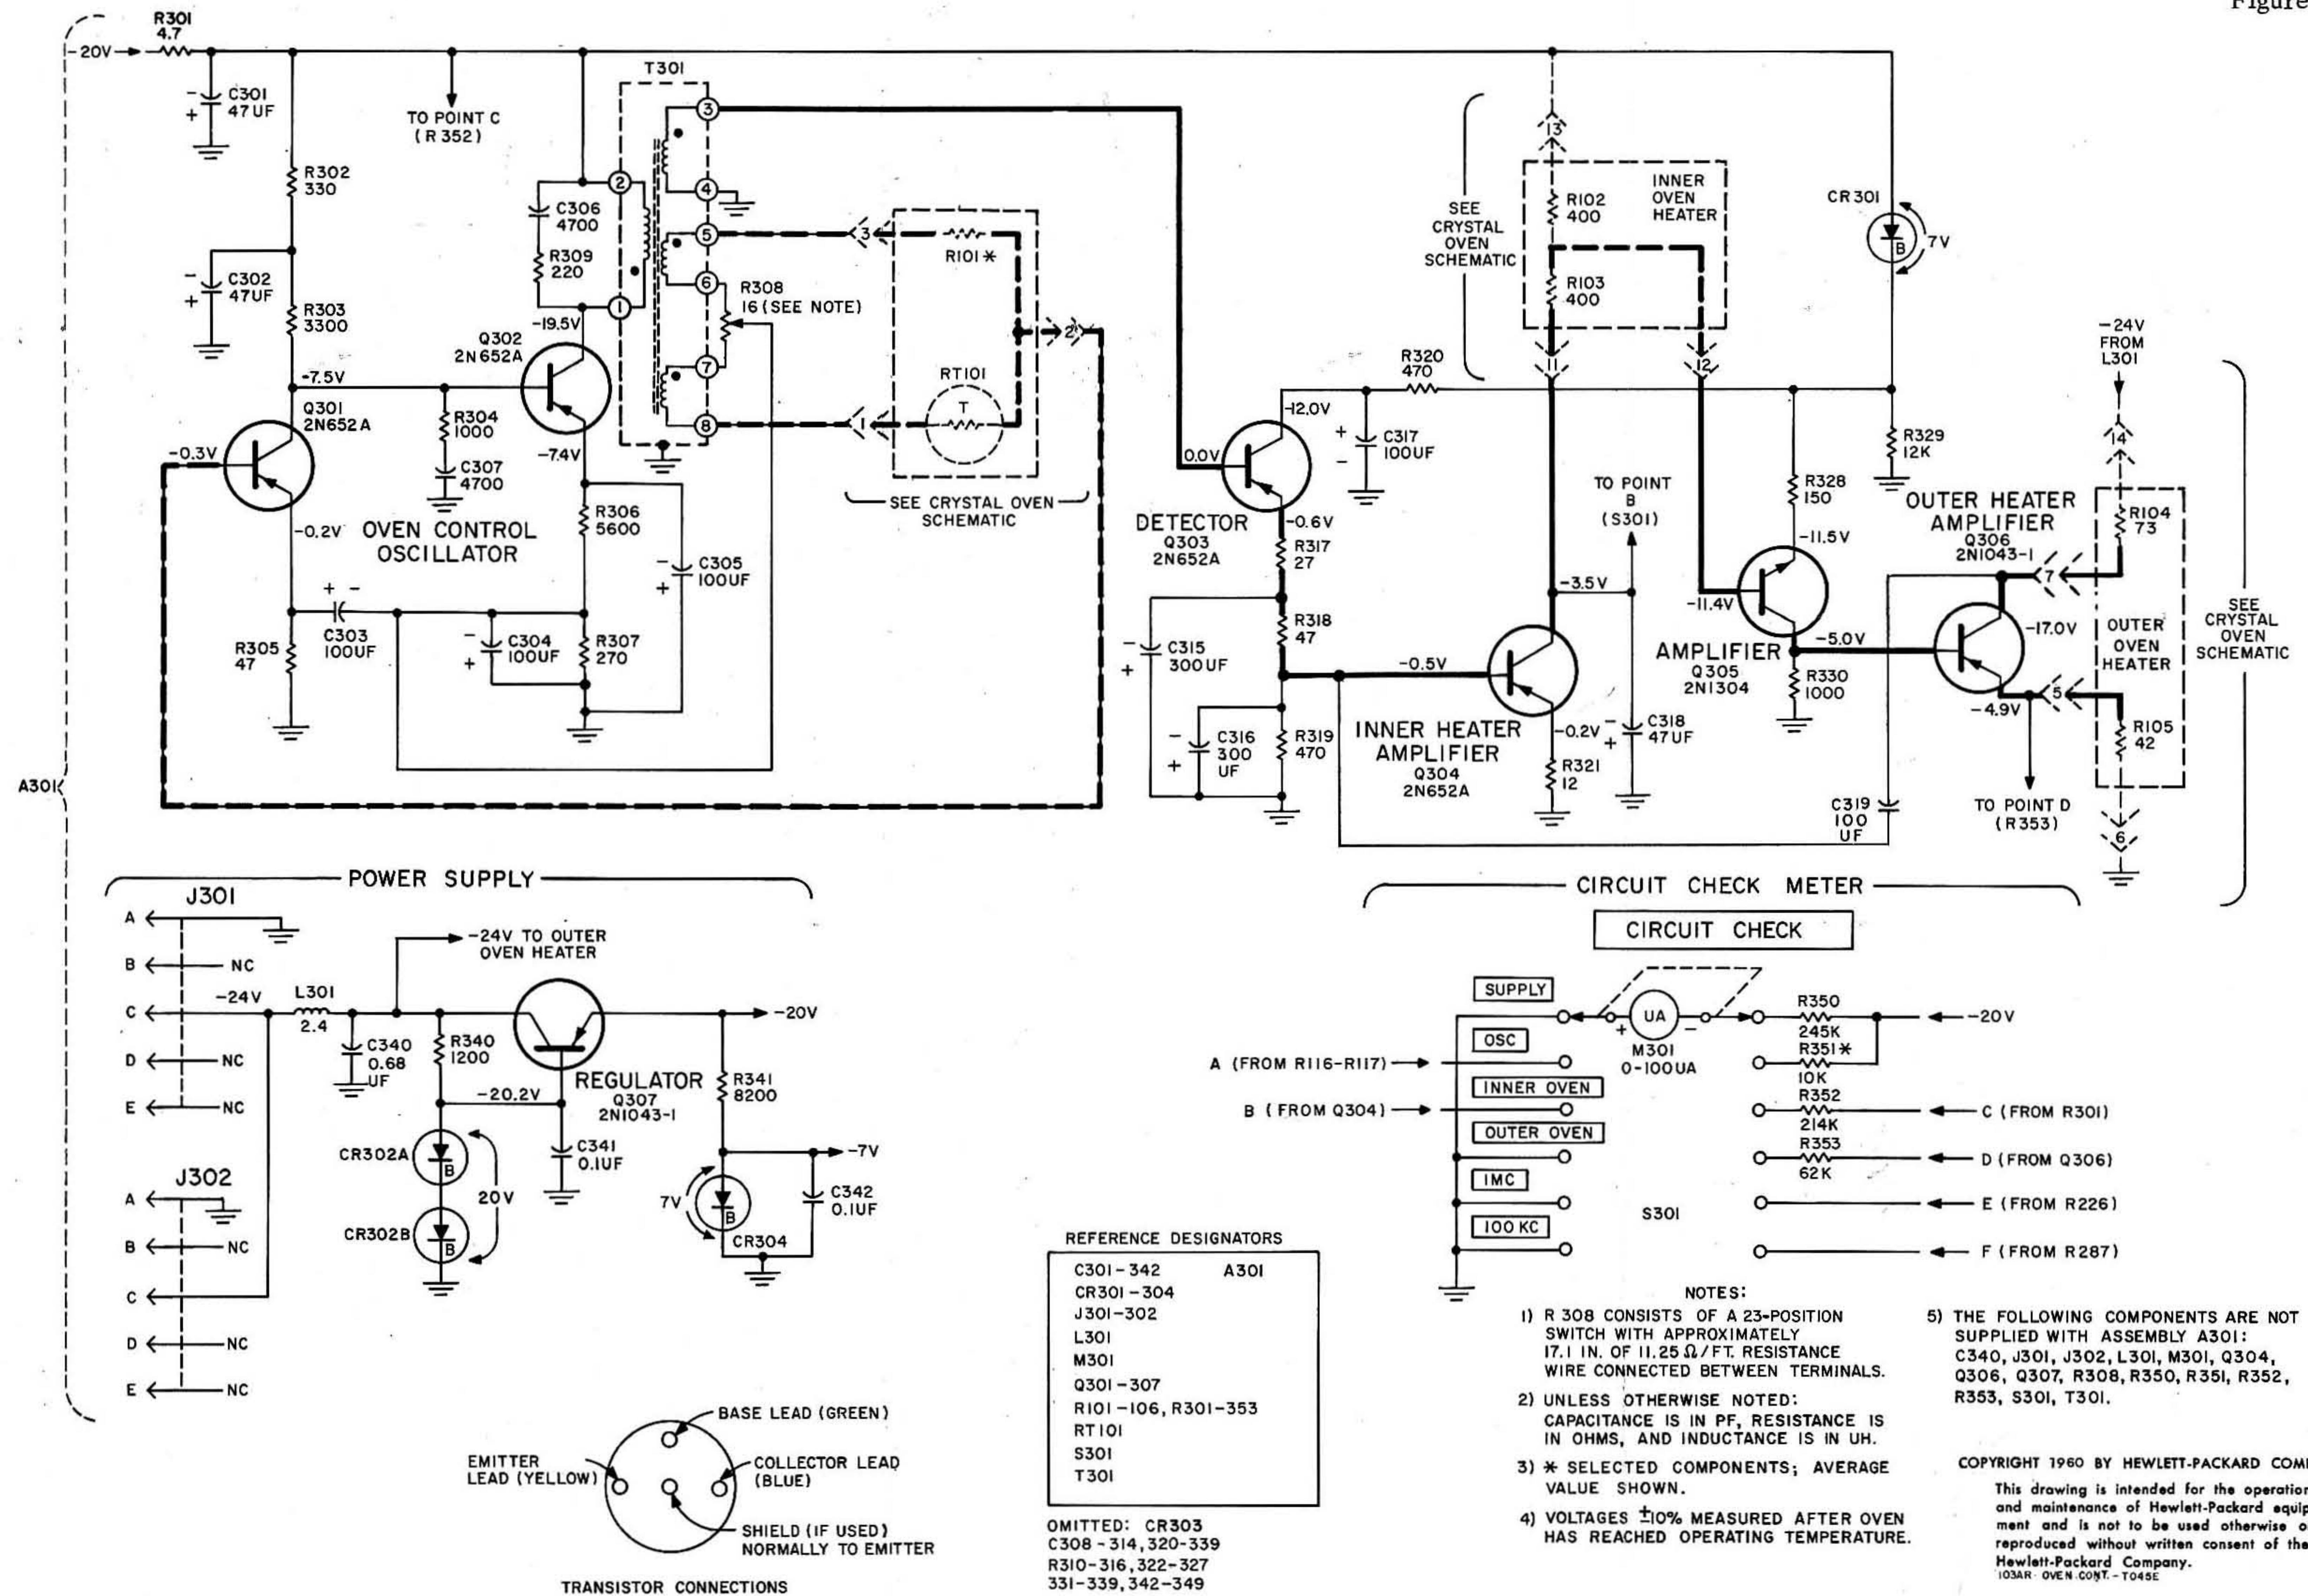


Figure 8-4. Oven Control

SECTION IX

REPLACEABLE PARTS

9-1. INTRODUCTION.

9-2. This section contains information for ordering replacement parts for the Model 103AR Quartz Oscillator.

9-3. Table 9-1 lists replaceable parts in alphabetical order of their reference designators. Detailed information on a part used more than once in the instrument is listed in table 9-2. Other reference designators applying to the same part refer to the initial designator. Miscellaneous parts are included in table 9-3. Detailed information includes the following:

- a. Reference designator.
- b. Full description of the part.
- c. Manufacturer of the part in a five-digit code; see list of manufacturers in appendix.
- d. Hewlett-Packard stock number.
- e. Total quantity used in the instrument (TQ col).
- f. Recommended spare quantity for complete maintenance during one year of isolated service (RS col).

9-4. ORDERING INFORMATION.

9-5. To order a replacement part, address order or inquiry either to your authorized Hewlett-Packard sales office or to

CUSTOMER SERVICE
Hewlett-Packard Company
395 Page Mill Road
Palo Alto, California

or, in Western Europe, to

Hewlett-Packard S. A.
Rue du Vieux Billard No. 1
Geneva, Switzerland

9-6. Specify the following information for each part:

- a. Model and complete serial number of instrument.
- b. Hewlett-Packard stock number.
- c. Circuit reference designator.
- d. Description.

9-7. To order a part not listed in table 9-1, give a complete description of the part and include its function and location.

Table 9-1. Reference Designator to Stock Number (Sheet 1 of 4)

Circuit Ref.	Stock No.	Note
A1 thru A100	Not assigned	
A101	103A-69A	
A102 thru A200	Not assigned	
A201	103A-60B	
A202	103A-60A	
A203	103A-60C	
A204	103A-60D	
A205	103A-60E	
A206	103A-9C	
A207 thru A300	Not assigned	
A301	103A-65A	
C1 thru C100	Not assigned	
C101	Part of A101	b
C102	Part of A101	b
C103	Part of A101	b
C104	Part of A101	b

Circuit Ref.	Stock No.	Note
C105	Part of A101	b
C106 thru C115	Not assigned	
C116	0170-0055	
C117	0121-0034	
C118 thru C119	Not assigned	
C120	0170-0038	
C121	0170-0055	
C122	0150-0012	
C123	0150-0012	
C124	0170-0055	
C125	0130-0012	
C126	0130-0011	
C127	0170-0055	
C128 thru C138	Not assigned	
C139	0150-0012	
C140	0150-0052	

b. Component not separately replaceable.

Table 9-1. Reference Designator to μ Stock Number (Sheet 4 of 4)

Circuit Ref.	μ Stock No.	Note	Circuit Ref.	μ Stock No.	Note
R256	0687-5621		R321	0687-1201	c
R257	0687-1231		R322 thru R327	Not assigned	
R258	0687-2221		R328	0687-1511	c
R259	0687-3321		R329	0687-1231	c
R260 thru R266	Not assigned		R330	0687-1021	c
R267	0687-4721		R331 thru R339	Not assigned	
R268	0687-2221		R340	0687-1221	c
R269	0687-3321		R341	0687-8221	c
R270	0687-1011		R342 thru R349	Not assigned	
R271 thru R274	Not assigned		R350	0730-0080	
R275	0687-1011		R351	0687-1031	a
R276	Not assigned		R352	0727-0222	
R277	0687-1821		R353	0730-0055	
R278	0727-0074		RT1 thru RT100	Not assigned	
R279	0727-0100		RT101	Part of A101	b
R280	0687-5601	a	S1 thru S200	Not assigned	
R281 thru R285	Not assigned		S201	3101-0014	
R286	0687-8211		S202 thru S300	Not assigned	
R287	0686-1635	a	S301	3100-0260	
R288 thru R300	Not assigned		T1 thru T100	Not assigned	
R301	0698-0001	c	T101	103A-9A	
R302	0687-3311	c	T102	103A-9B	
R303	0687-3321	c	T103 thru T200	Not assigned	
R304	0687-1021	c	T201	Part of A201	b
R305	0687-4701	c	T202	Part of A202	b
R306	0687-5621	c	T203	Part of A203	b
R307	0687-2711	c	T204	Part of A204	b
R308	3100-0261	c	T205	Part of A206	b
R309	0687-2211	c	T206 thru T300	Not assigned	
R310	0687-4701	c	T301	103A-9D	
R311 thru R316	Not assigned		XT1 thru XT100	Not assigned	
R317	0687-2701	c	XT101	1200-0017	
R318	0687-4701	c	XT102	1200-0017	
R319	0687-4711	c	Y1 thru Y100	Not assigned	
R320	0687-4711	c	Y101	Part of A101	b

a. Optimum value selected at factory. Average value shown.

b. Component not separately replaceable.

c. Part of A301. Component is separately replaceable or may be replaced with assembly.

Table 9-2, Electrical Components (Sheet 1 of 5)

Stock No	Description	Mfr *		TQ*	RS*		
103A-7A	Assembly, Capacitor, sealed	28480		1	1		
103A-9A	Transformer: AGC Interstage	28480		1	1		
103A-9B	Transformer: AGC Output Interstage	28480		1	1		
103A-9C	Assembly, transformer: 100 kc Output (includes C264, T205)	28480		1	1		
103A-9D	Assembly, transformer: Oven Control	28480		1	1		
103A-60A	Assembly, transformer: 1 mc Output (includes C212, T202)	28480		1	1		
103A-60B	Assembly, transformer: 1 mc Buffer (includes C204, C205, T201)	28480		1	1		
103A-60C	Assembly, transformer: Divider Buffer (includes C223, T203)	28480		1	1		
103A-60D	Assembly, transformer: 900 kc Mult. (includes C243, T204)	28480		1	1		
103A-60E	Assembly, filter: 100 kc (includes C234, C251, L202, L203)	28480		1	1		
103A-65A	Assembly, Oven Control Circuit Board (includes C301-C307 Q301-Q303 C315-C318 Q305 C341 R301-R307 C342 R309 CR301 R317-R321 CR302A, B R328-R330 CR304 R340 R341)	28480		1	1		
103A-69A	Assembly, Crystal Oven (includes C101 P103 C102 Q101 C104 R106 C105 RT101 J101 Y101 J102)	28480		1	1		
103A-16D	Connector: includes coaxial cable	28480		1	1		
103A-16E	Connector: includes coaxial cable	28480		1	1		
0130-0011	Capacitor: variable, ceramic, 1.5-7 pf	72982		1	1		
0130-0012	Capacitor: variable, ceramic, 5-25 pf	72982		1	1		
0140-0007	Capacitor: fixed, mica, 680 pf ±10%, 500 vdcw	76433		1	1		

* See introduction to this section

Table 9-2. Replaceable Parts (Sheet 2 of 5)

Ckt Ref.	Description	Mfr *		TQ*	RS*		
0140-0008	Capacitor: fixed, mica, 0.01 μ f \pm 10%, 300 vdcw	76433		1	1		
0140-0009	Capacitor: fixed, mica, 0.01 μ f \pm 5%, 500 vdcw	00656		1	1		
0140-0162	Capacitor: fixed, mica, 4700 pf \pm 10%, 300 vdcw	72136		2	1		
0140-0164	Capacitor: fixed, mica, 6800 pf \pm 5%, 500 vdcw	72136		1	1		
0150-0012	Capacitor: fixed, ceramic, 0.01 μ f \pm 20%, 1000 vdcw	71590		14	4		
0150-0052	Capacitor: fixed, ceramic, 0.05 μ f \pm 20%, 400 vdcw	05729		4	1		
0150-0084	Capacitor: fixed, ceramic, 0.1 μ f -20% +80%, 50 vdcw	56289		1	1		
0170-0024	Capacitor: fixed, mylar, 0.022 μ f \pm 20%, 200 vdcw	56289		1	1		
0170-0038	Capacitor: fixed, mylar, 0.22 μ f \pm 10%, 200 vdcw	56289		5	2		
0170-0039	Capacitor: fixed, mylar, 0.68 μ f \pm 10%, 100 vdcw	84411		1	1		
0170-0055	Capacitor: fixed, mylar, 0.1 μ f \pm 20%, 100 vdcw	56289		9	2		
0170-0066	Capacitor: fixed, mylar, 0.027 μ f \pm 10%, 200 vdcw	56289		1	1		
0180-0083	Capacitor: fixed, tantalum electrolytic, 100 μ f -15% + 20%, 6 vdcw	10411		1	1		
0180-0084	Capacitor: fixed, tantalum electrolytic, 300 μ f -15% +20%, 6 vdcw	10411		2	1		
0180-0097	Capacitor: fixed, tantalum electrolytic, 47 μ f \pm 10%, 35 vdcw	56289		3	1		
0180-0098	Capacitor: fixed, tantalum electrolytic, 100 μ f \pm 20%, 20 vdcw	56289		3	1		
0180-0113	Capacitor: fixed, tantalum electrolytic 100 μ f, + 5% -15%, 30 vdcw	56289		1	1		
0686-1535	Resistor: fixed, composition, 15,000 ohms \pm 5%, 1/2 W	01121		1	1		
0686-1635	Resistor: fixed, composition, 16,000 ohms \pm 5%, 1/2 W	01121		1	1		

* See introduction to this section

Table 9-2. Replaceable Parts (Sheet 3 of 5)

Ckt Ref.	Description	Mfr *		TQ*	RS*		
0687-1011	Resistor: fixed, composition, 100 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-1021	Resistor: fixed, composition, 1000 ohms $\pm 10\%$, 1/2 W	01121		7	2		
0687-1031	Resistor: fixed, composition, 10,000 ohms $\pm 10\%$, 1/2 W	01121		5	2		
0687-1201	Resistor: fixed, composition, 12 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-1221	Resistor: fixed, composition, 1200 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-1231	Resistor: fixed, composition, 12,000 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-1511	Resistor: fixed, composition, 150 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-1821	Resistor: fixed, composition, 1800 ohms $\pm 10\%$, 1/2 W	01121		5	2		
0687-1831	Resistor: fixed, composition, 18,000 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-2201	Resistor: fixed, composition, 22 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-2211	Resistor: fixed, composition, 220 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-2221	Resistor: fixed, composition, 2200 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-2231	Resistor: fixed, composition, 22,000 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-2701	Resistor: fixed, composition, 27 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-2711	Resistor: fixed, composition, 270 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-3301	Resistor: fixed, composition, 33 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-3311	Resistor: fixed, composition, 330 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-3321	Resistor: fixed, composition, 3300 ohms $\pm 10\%$, 1/2 W	01121		6	2		
0687-3921	Resistor: fixed, composition, 3900 ohms $\pm 10\%$, 1/2 W	01121		1	1		

* See introduction to this section

Table 9-2. Replaceable Parts (Sheet 4 of 5)

Ckt Ref.	Description	Mfr *		TQ*	RS*		
0687-4701	Resistor: fixed, composition, 47 ohms $\pm 10\%$, 1/2 W	01121		6	2		
0687-4711	Resistor: fixed, composition, 470 ohms $\pm 10\%$, 1/2 W	01121		3	1		
0687-4721	Resistor: fixed, composition, 4700 ohms $\pm 10\%$, 1/2 W	01121		4	1		
0687-5601	Resistor: fixed, composition, 56 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-5621	Resistor: fixed, composition, 5600 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-5631	Resistor: fixed, composition, 56,000 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0687-8211	Resistor: fixed, composition, 820 ohms $\pm 10\%$, 1/2 W	01121		2	1		
0687-8221	Resistor: fixed, composition, 8200 ohms $\pm 10\%$, 1/2 W	01121		1	1		
0698-0001	Resistor: fixed, composition, 4.7 ohms $\pm 5\%$, 1/2 W	01121		1	1		
0727-0004	Resistor: fixed, deposited carbon, 5 ohms $\pm 1\%$, 1/2 W	19701		1	1		
0727-0074	Resistor: fixed, deposited carbon, 436 ohms $\pm 1/2\%$, 1/2 W	19701		2	1		
0727-0100	Resistor: fixed, deposited carbon, 1000 ohms $\pm 1\%$, 1/2 W	19701		2	1		
0727-0123	Resistor: fixed, deposited carbon, 2900 ohms $\pm 1\%$, 1/2 W	19701		1	1		
0727-0222	Resistor: fixed, deposited carbon, 214,000 ohms $\pm 1\%$, 1/2 W	19701		1	1		
0730-0055	Resistor: fixed, deposited carbon, 62,000 ohms $\pm 1\%$, 1 W	19701		1	1		
0730-0080	Resistor: fixed, deposited carbon, 245,000 ohms $\pm 1\%$, 1 W	19701		1	1		
1120-0083	Meter: 0-100 μ amps	81030		1	1		
1200-0017	Socket, tube: 7 pin	71785		2	1		

* See introduction to this section

Table 9-2. Electrical Components (Sheet 5 of 5)

hp Stock No.	Description	Mfr *		TQ*	RS*		
1250-0083	Connector: female, BNC, UG1094/U	91737		1	1		
1250-0109	Connector: coaxial cable plug	98278		2	1		
1251-0111	Connector: male, 5 pin	71468		2	1		
1251-0143	Connector: female, 14 pin	02660		1	1		
1850-0029	Transistor: 2N384, specially selected for hp type 1850-0029	28480		4	4		
1850-0037	Transistor: 2N274	02735		6	6		
1850-0054	Transistor: 2N652A	04713		4	4		
1850-0061	Transistor: 2N1043	01295		2	2		
1851-0017	Transistor: 2N1304	01295		1	1		
1902-0006	Diode, silicon: avalanche	01281		1	1		
1902-0007	Diode, silicon: avalanche series, matched pair	04713		1	1		
1902-0008	Diode, silicon: avalanche	81483		1	1		
1910-0011	Diode, germanium	73293		5	5		
3100-0260	Switch, rotary: 1 section, 6 position	76854		1	1		
3100-0261	Switch, rotary: 1 section, 23 position	76854		1	1		
3101-0014	Switch, Push: SPDT	82389		1	1		
9140-0001	Inductor, fixed: 2.3 μ h	0000M		1	1		
9140-0019	Inductor, fixed: 200 μ h	99848		1	1		
9140-0022	Inductor, fixed: 500 μ h	99848		1	1		
9140-0124	Inductor, fixed: 10 μ h	98734		1	1		



* See introduction to this section

Table 9-3. Miscellaneous Components (Sheet 1 of 1)

Ckt Ref.	Description	Mfr *	hp Stock No.	TQ*	RS*		
	Cable, power	28480	103A-16A	1	1		
	Connector, female: 5 pin MS 3106E-14S-5S (mates with J301, J302)	71468	1251-0126	1	1		
	Connector, male: 11 pin (mates with power output connector on hp Model 724A/B)	02660	1251-0052	1	1		
	Counter, direct drive	79142	1140-0003	1	1		
	Ball, stainless steel	76210	1410-0086	1	1		
	Bearing, surface	28480	103A-17A	1	1		
	Knob	28480	G-74N	1	1		
	Shield, tube (for XT101, XT102)	71785	1220-0011	2	0		
	Spring	91260	1460-0023		1		
	Retainer	28480	103A-17B	1	1		

* See introduction to this section

Model 103AR

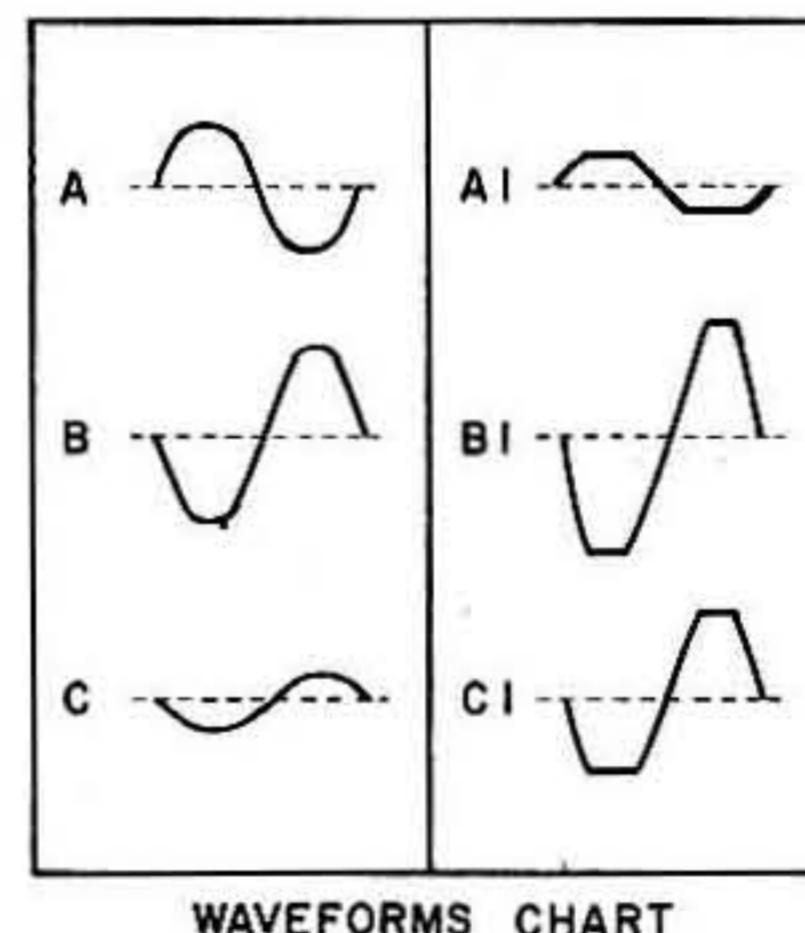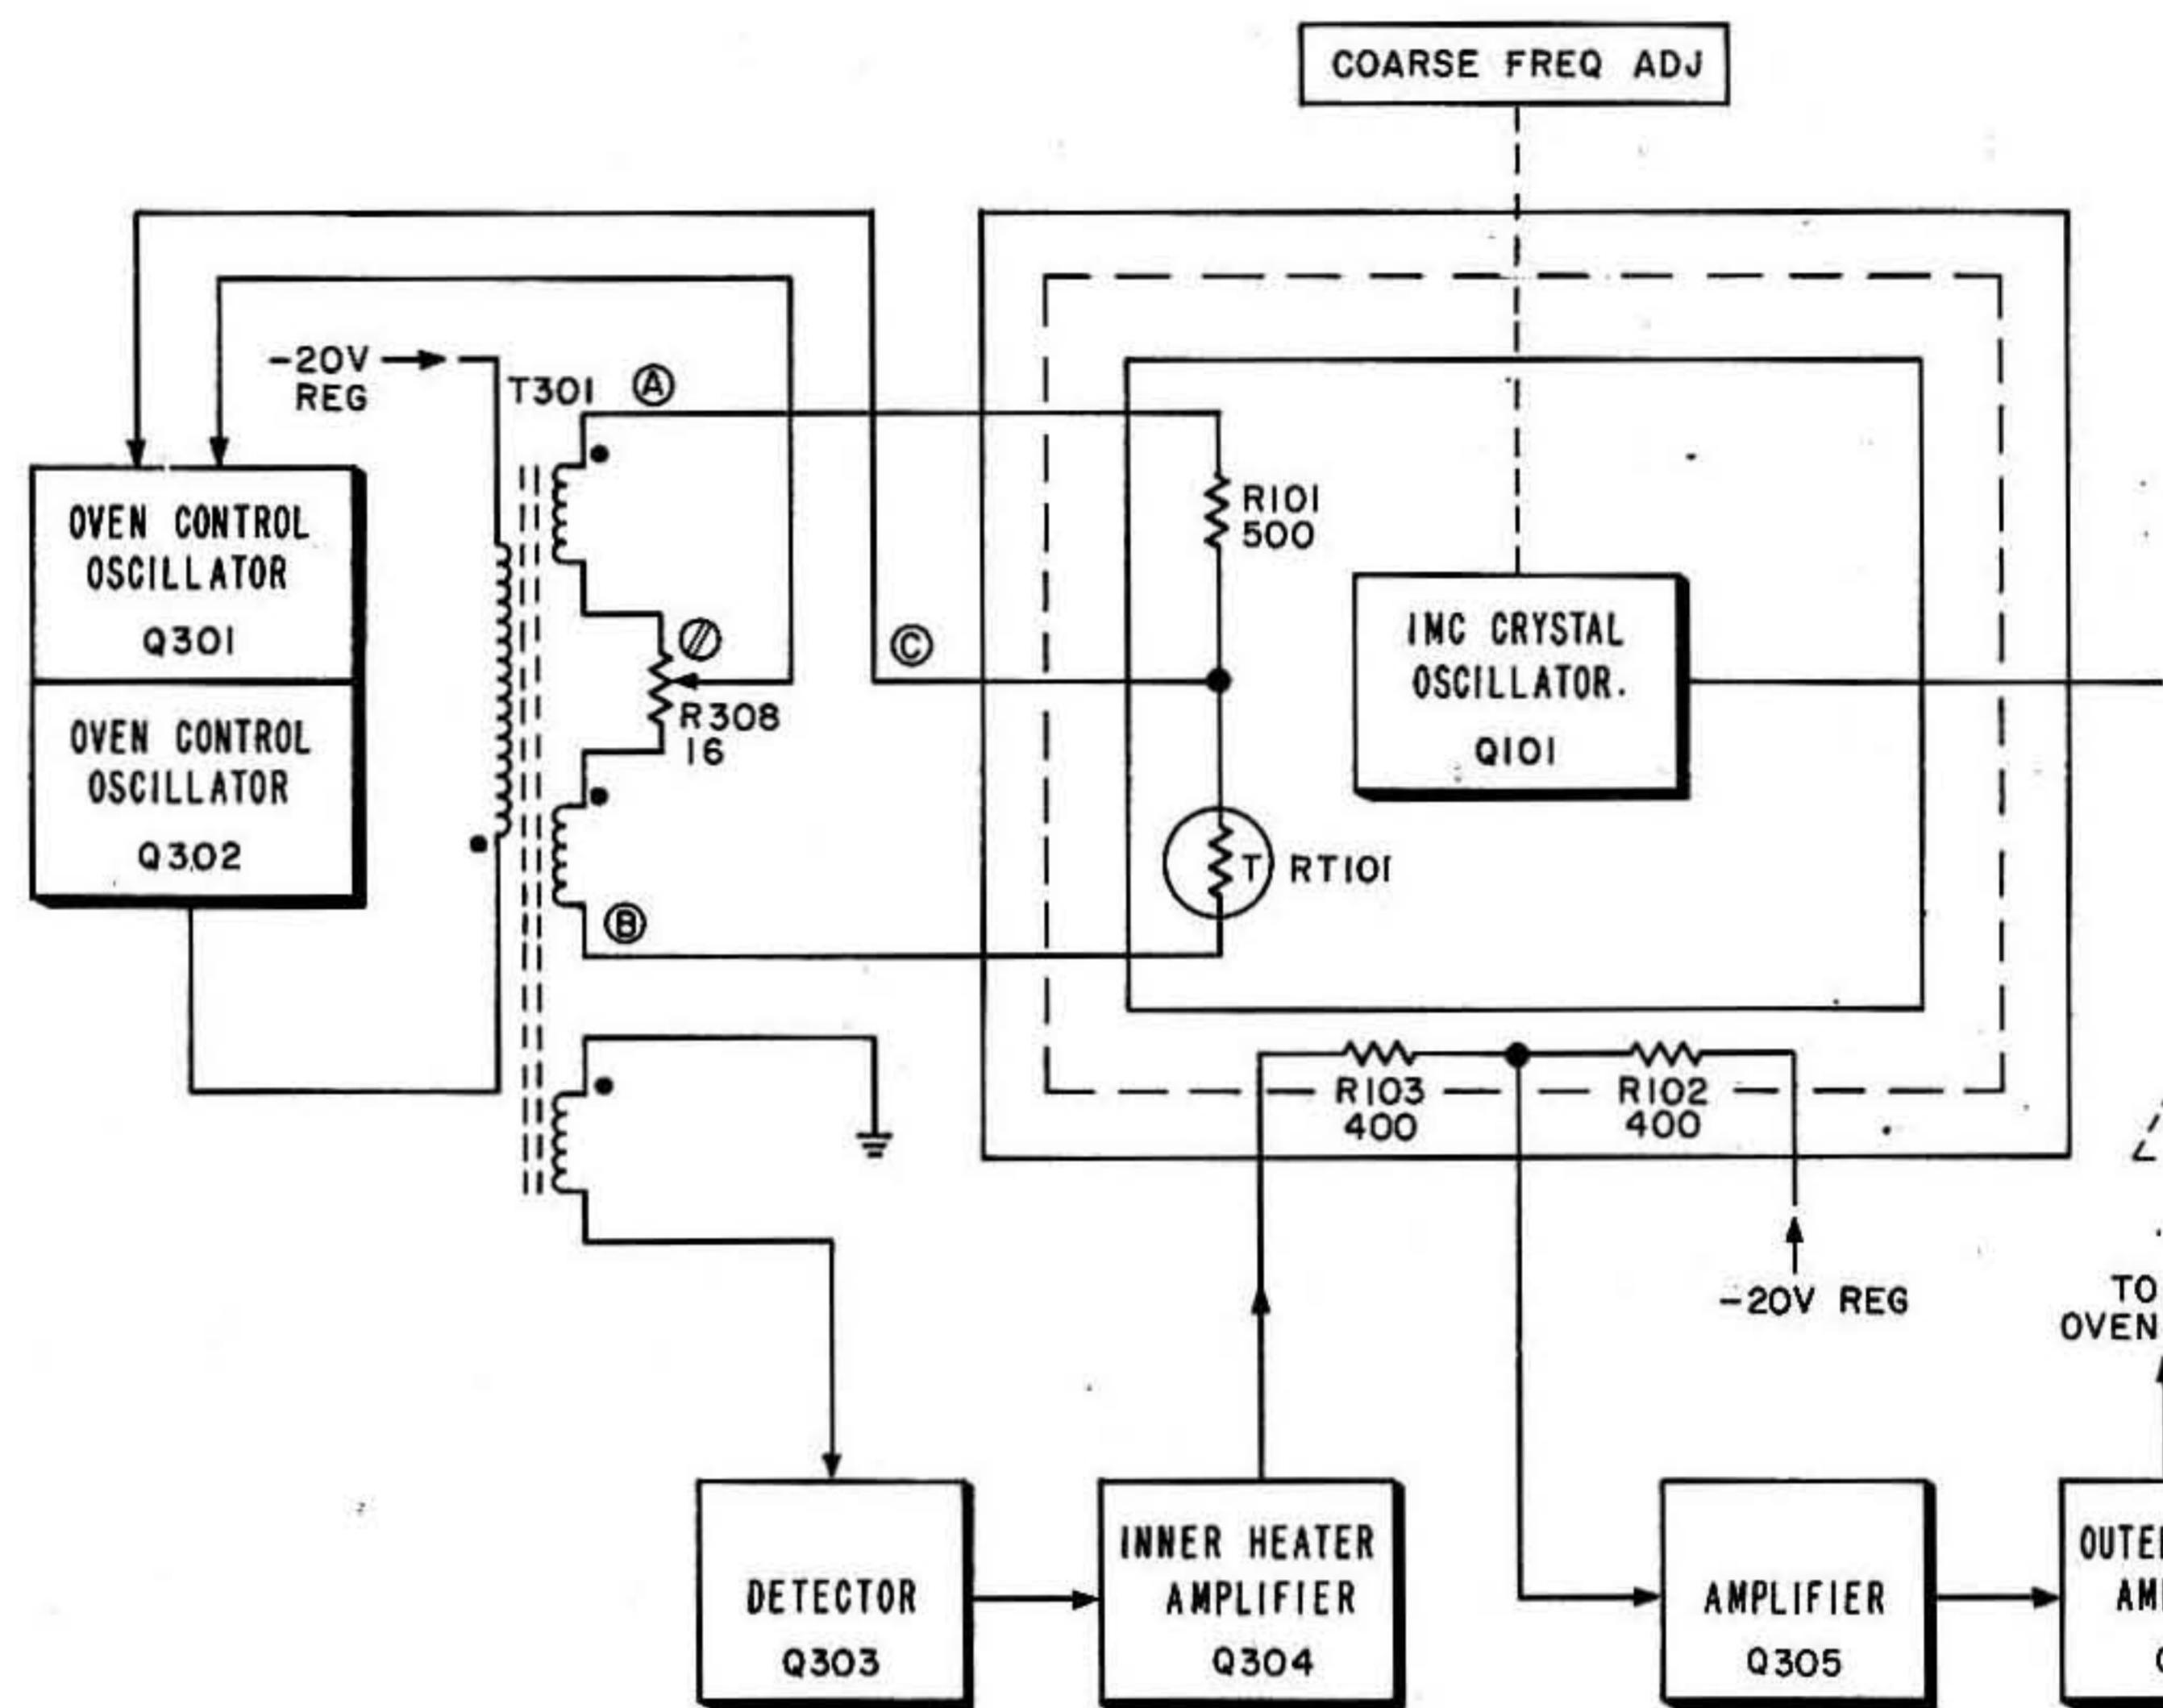

WAVEFORMS CHART



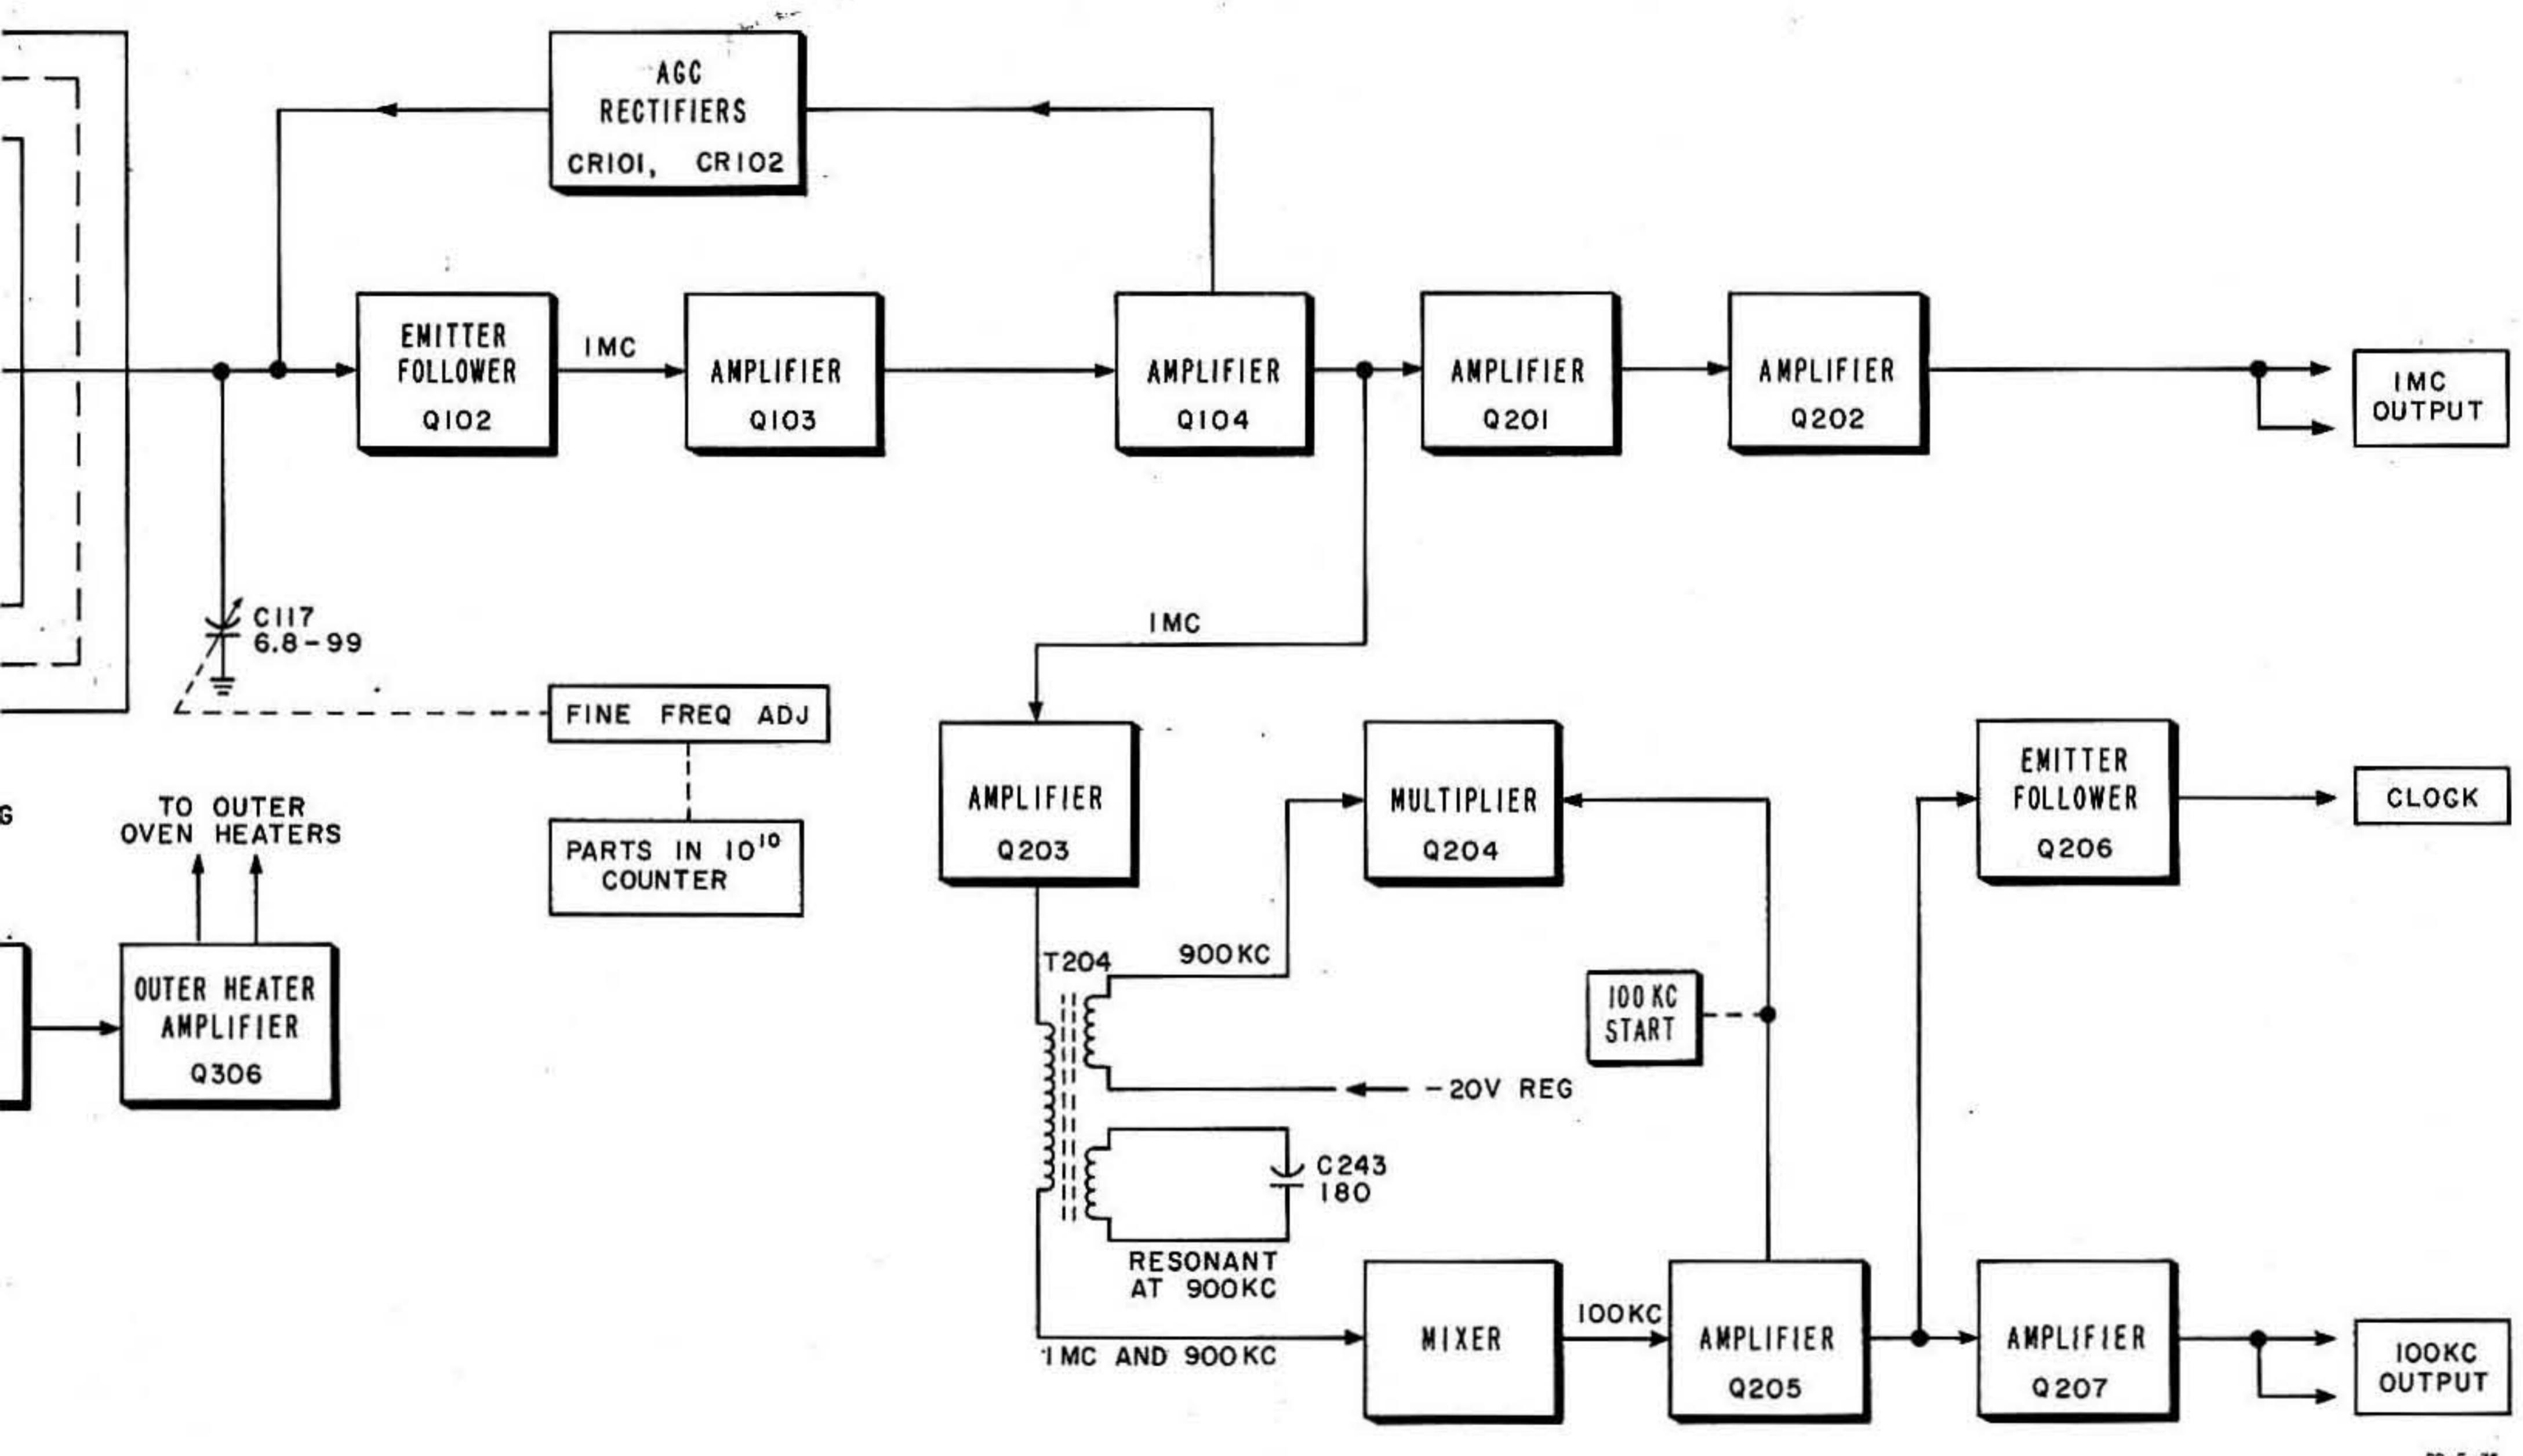


Figure 5-2. Functional Diagram

Model 103AR

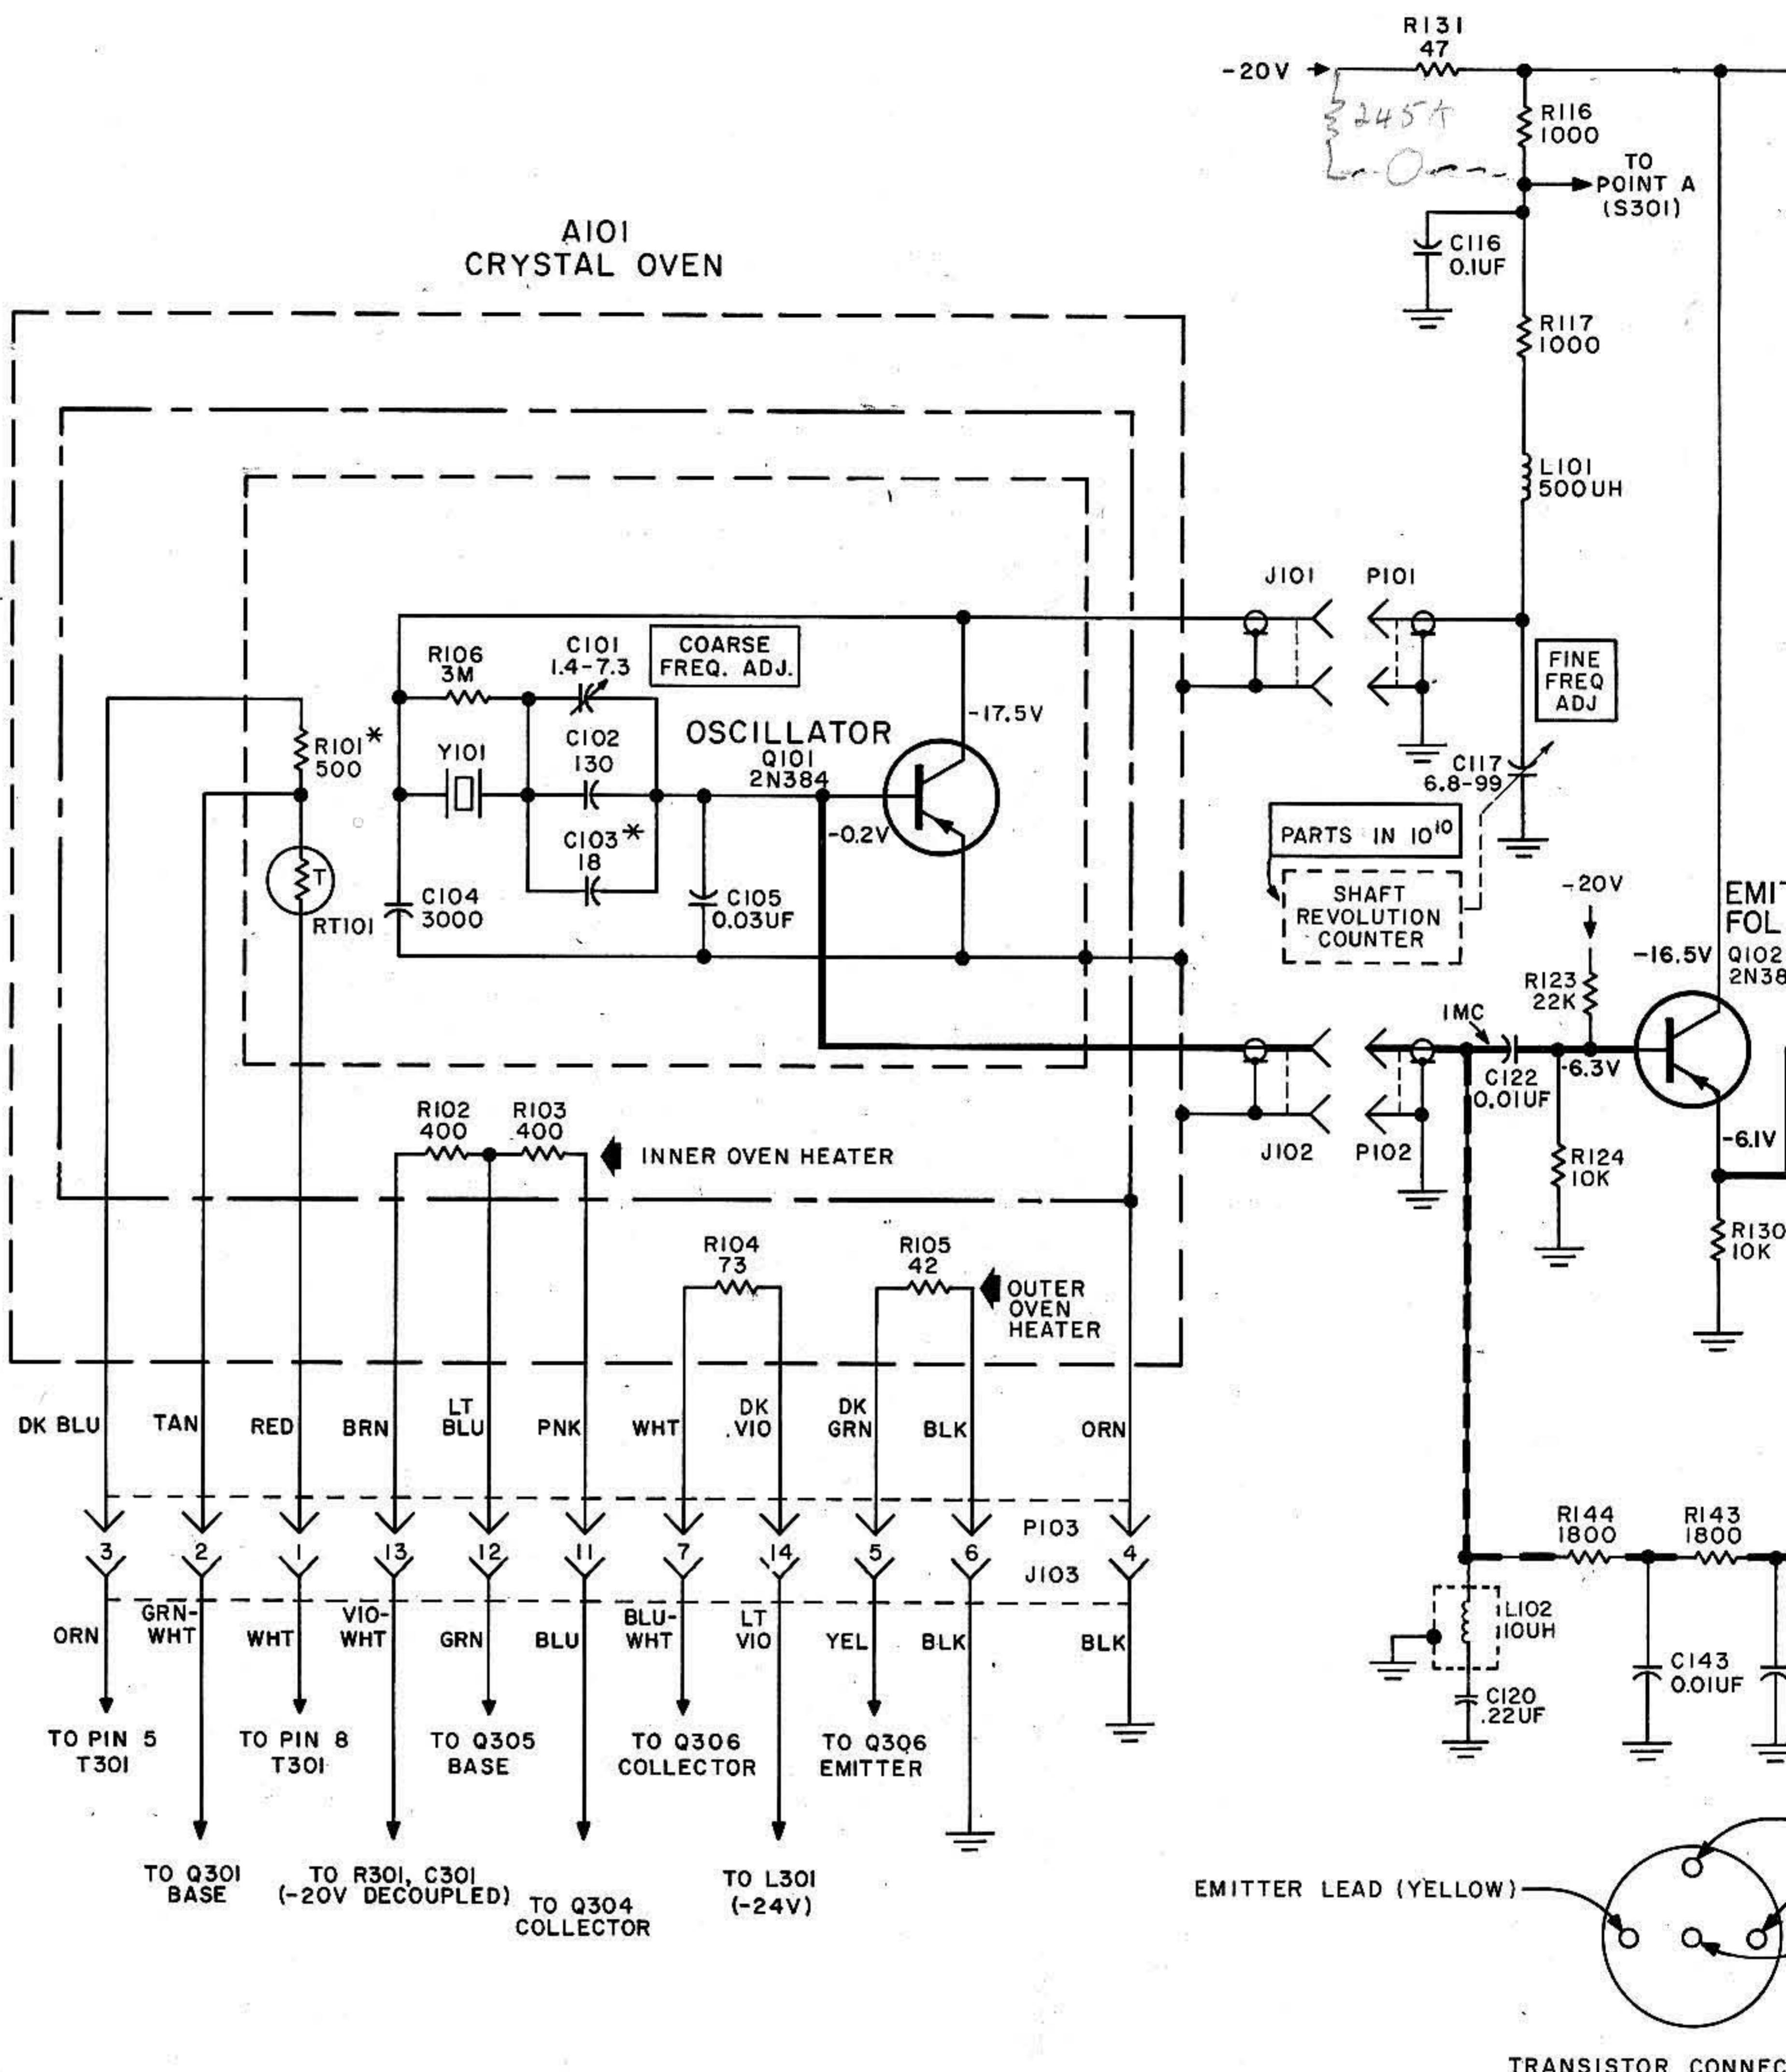

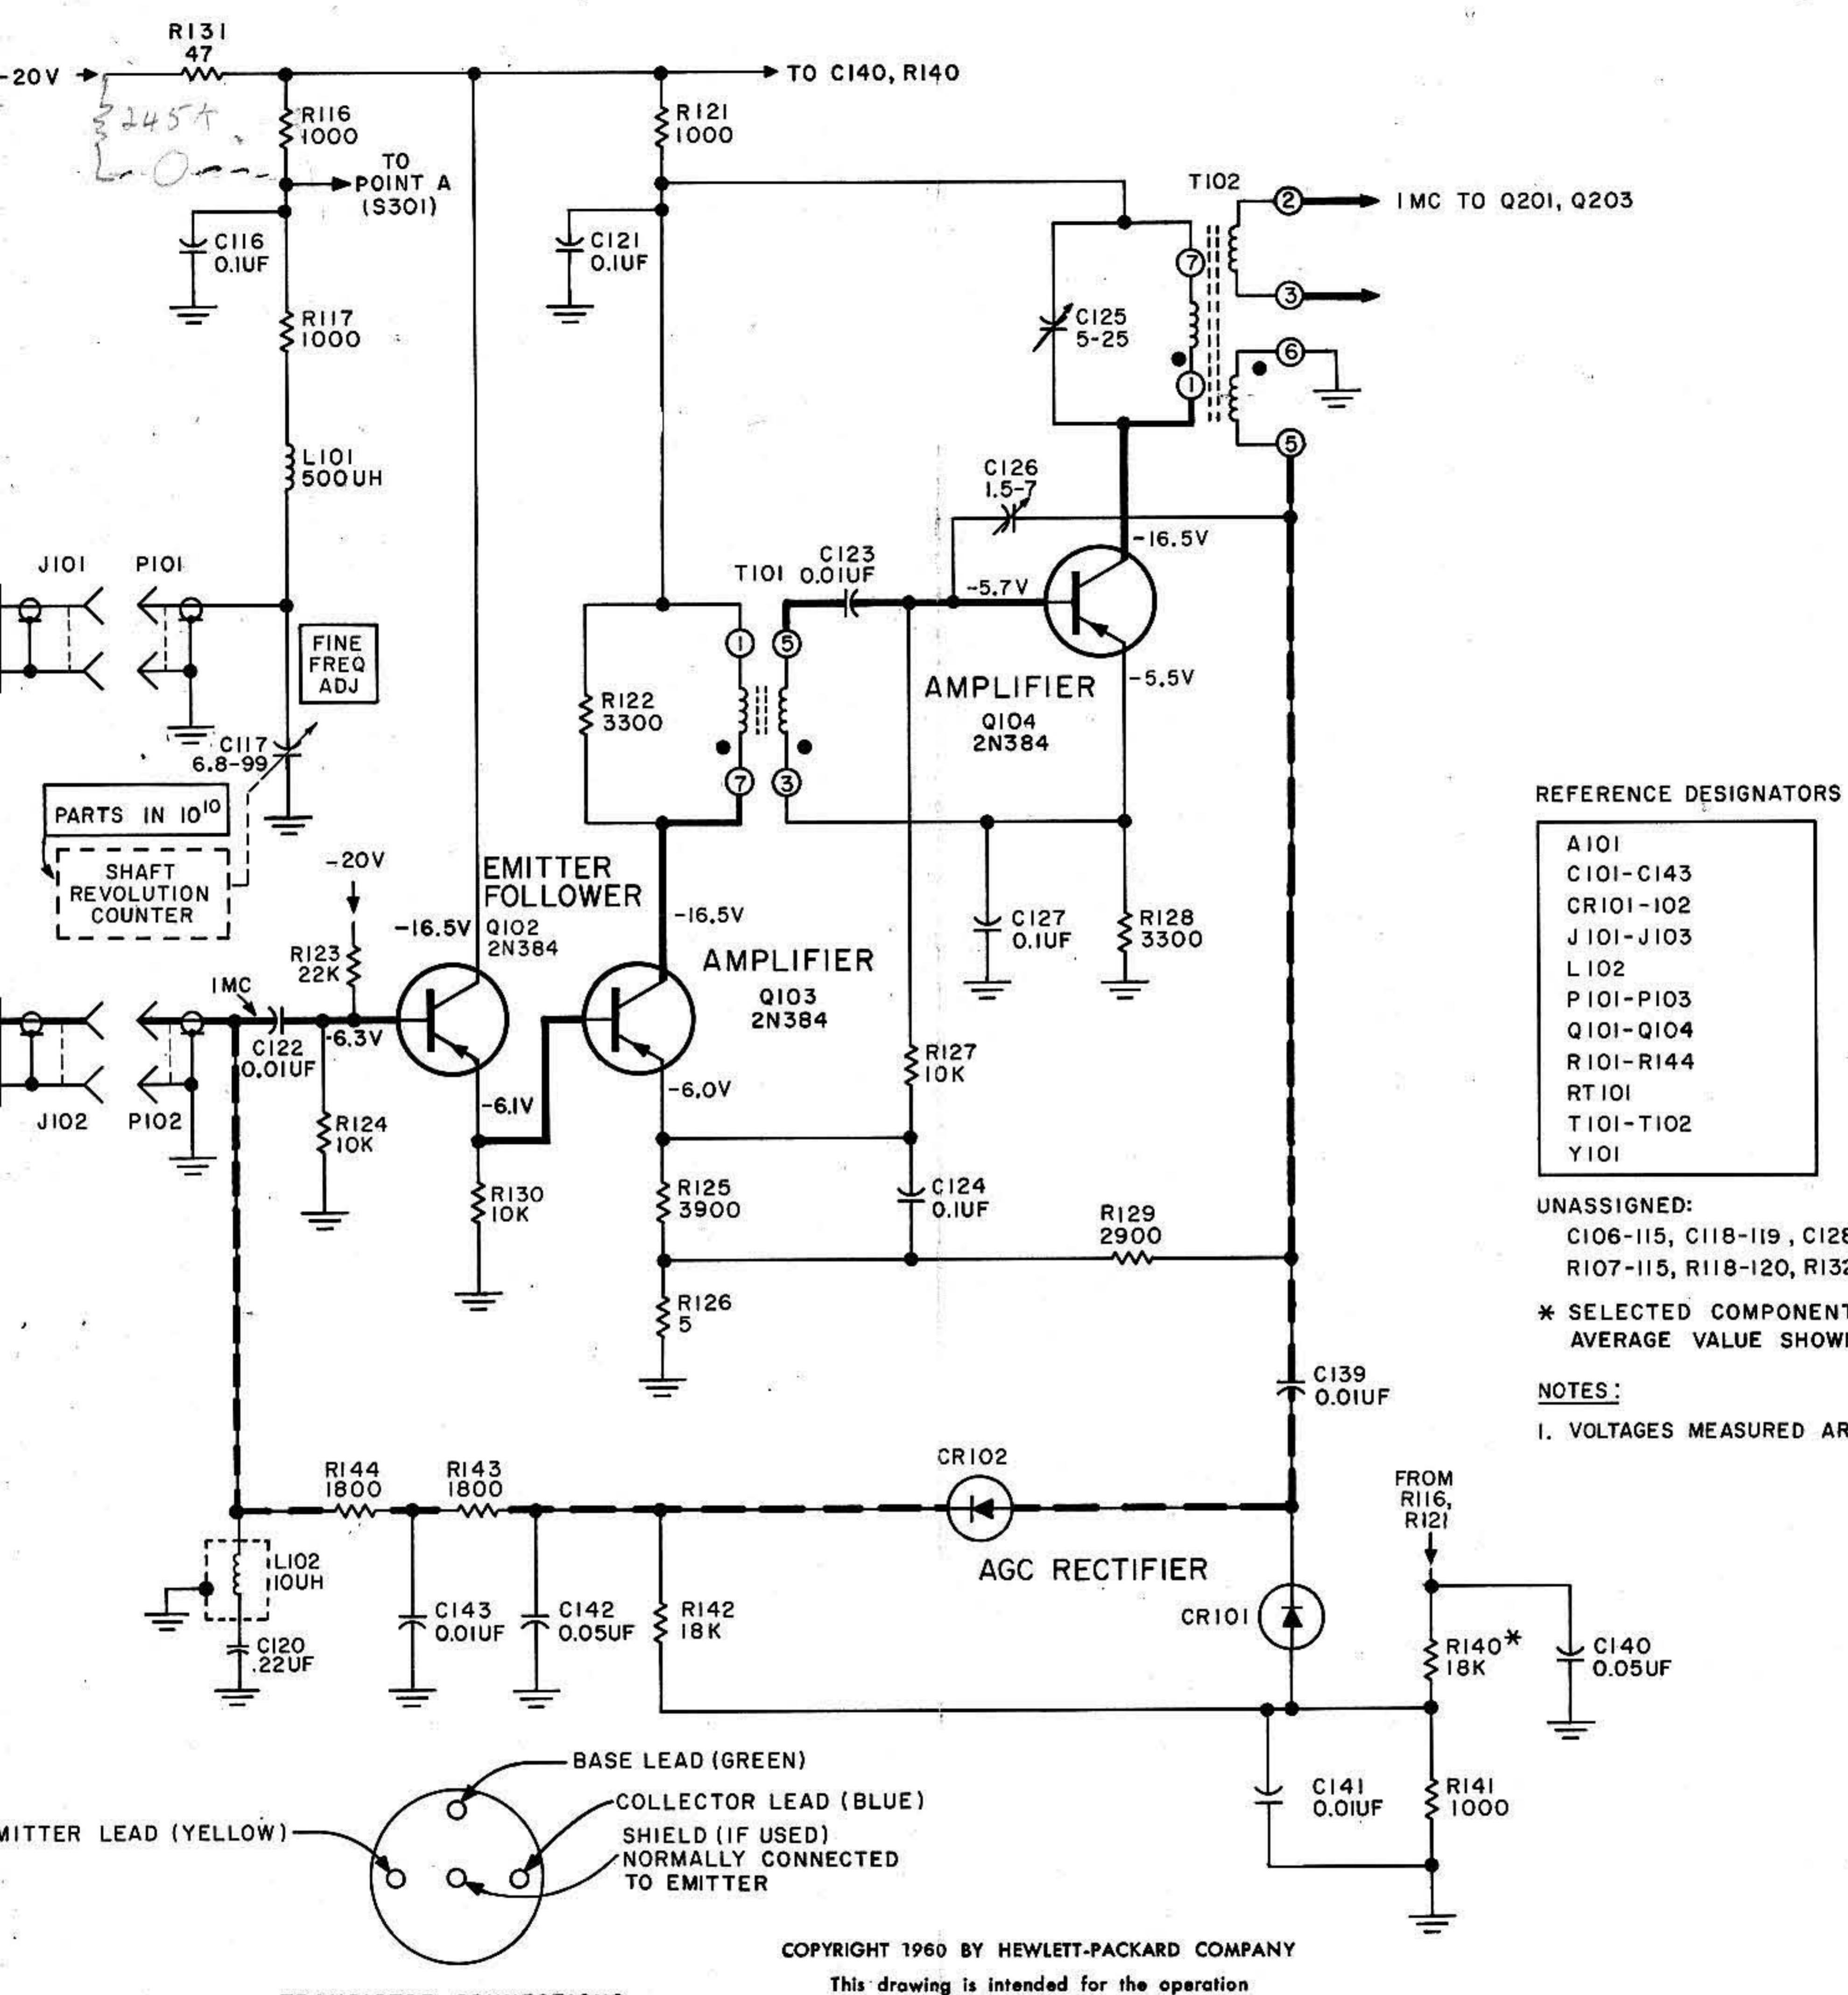

REFERENCE DESIGNATORS

A101
C101-C143
CRI01-I02
J101-J103
L102
P101-P103
Q101-Q104
R101-R144
RT101
T101-T102
Y101

UNASSIGNED:
C106-II5, C118-II9, C128-I38
R107-II5, R118-I20, R132-I39

* SELECTED COMPONENT;
AVERAGE VALUE SHOWN

NOTES:


I. VOLTAGES MEASURED ARE $\pm 10\%$


COPYRIGHT 1960 BY HEWLETT-PACKARD COMPANY

This drawing is intended for the operation
and maintenance of Hewlett-Packard equipment
and is not to be used otherwise or
reproduced without written consent of the
Hewlett-Packard Company. 103AR - OSC-T135A

Figure 8-2. Oscillator


Model 103AR

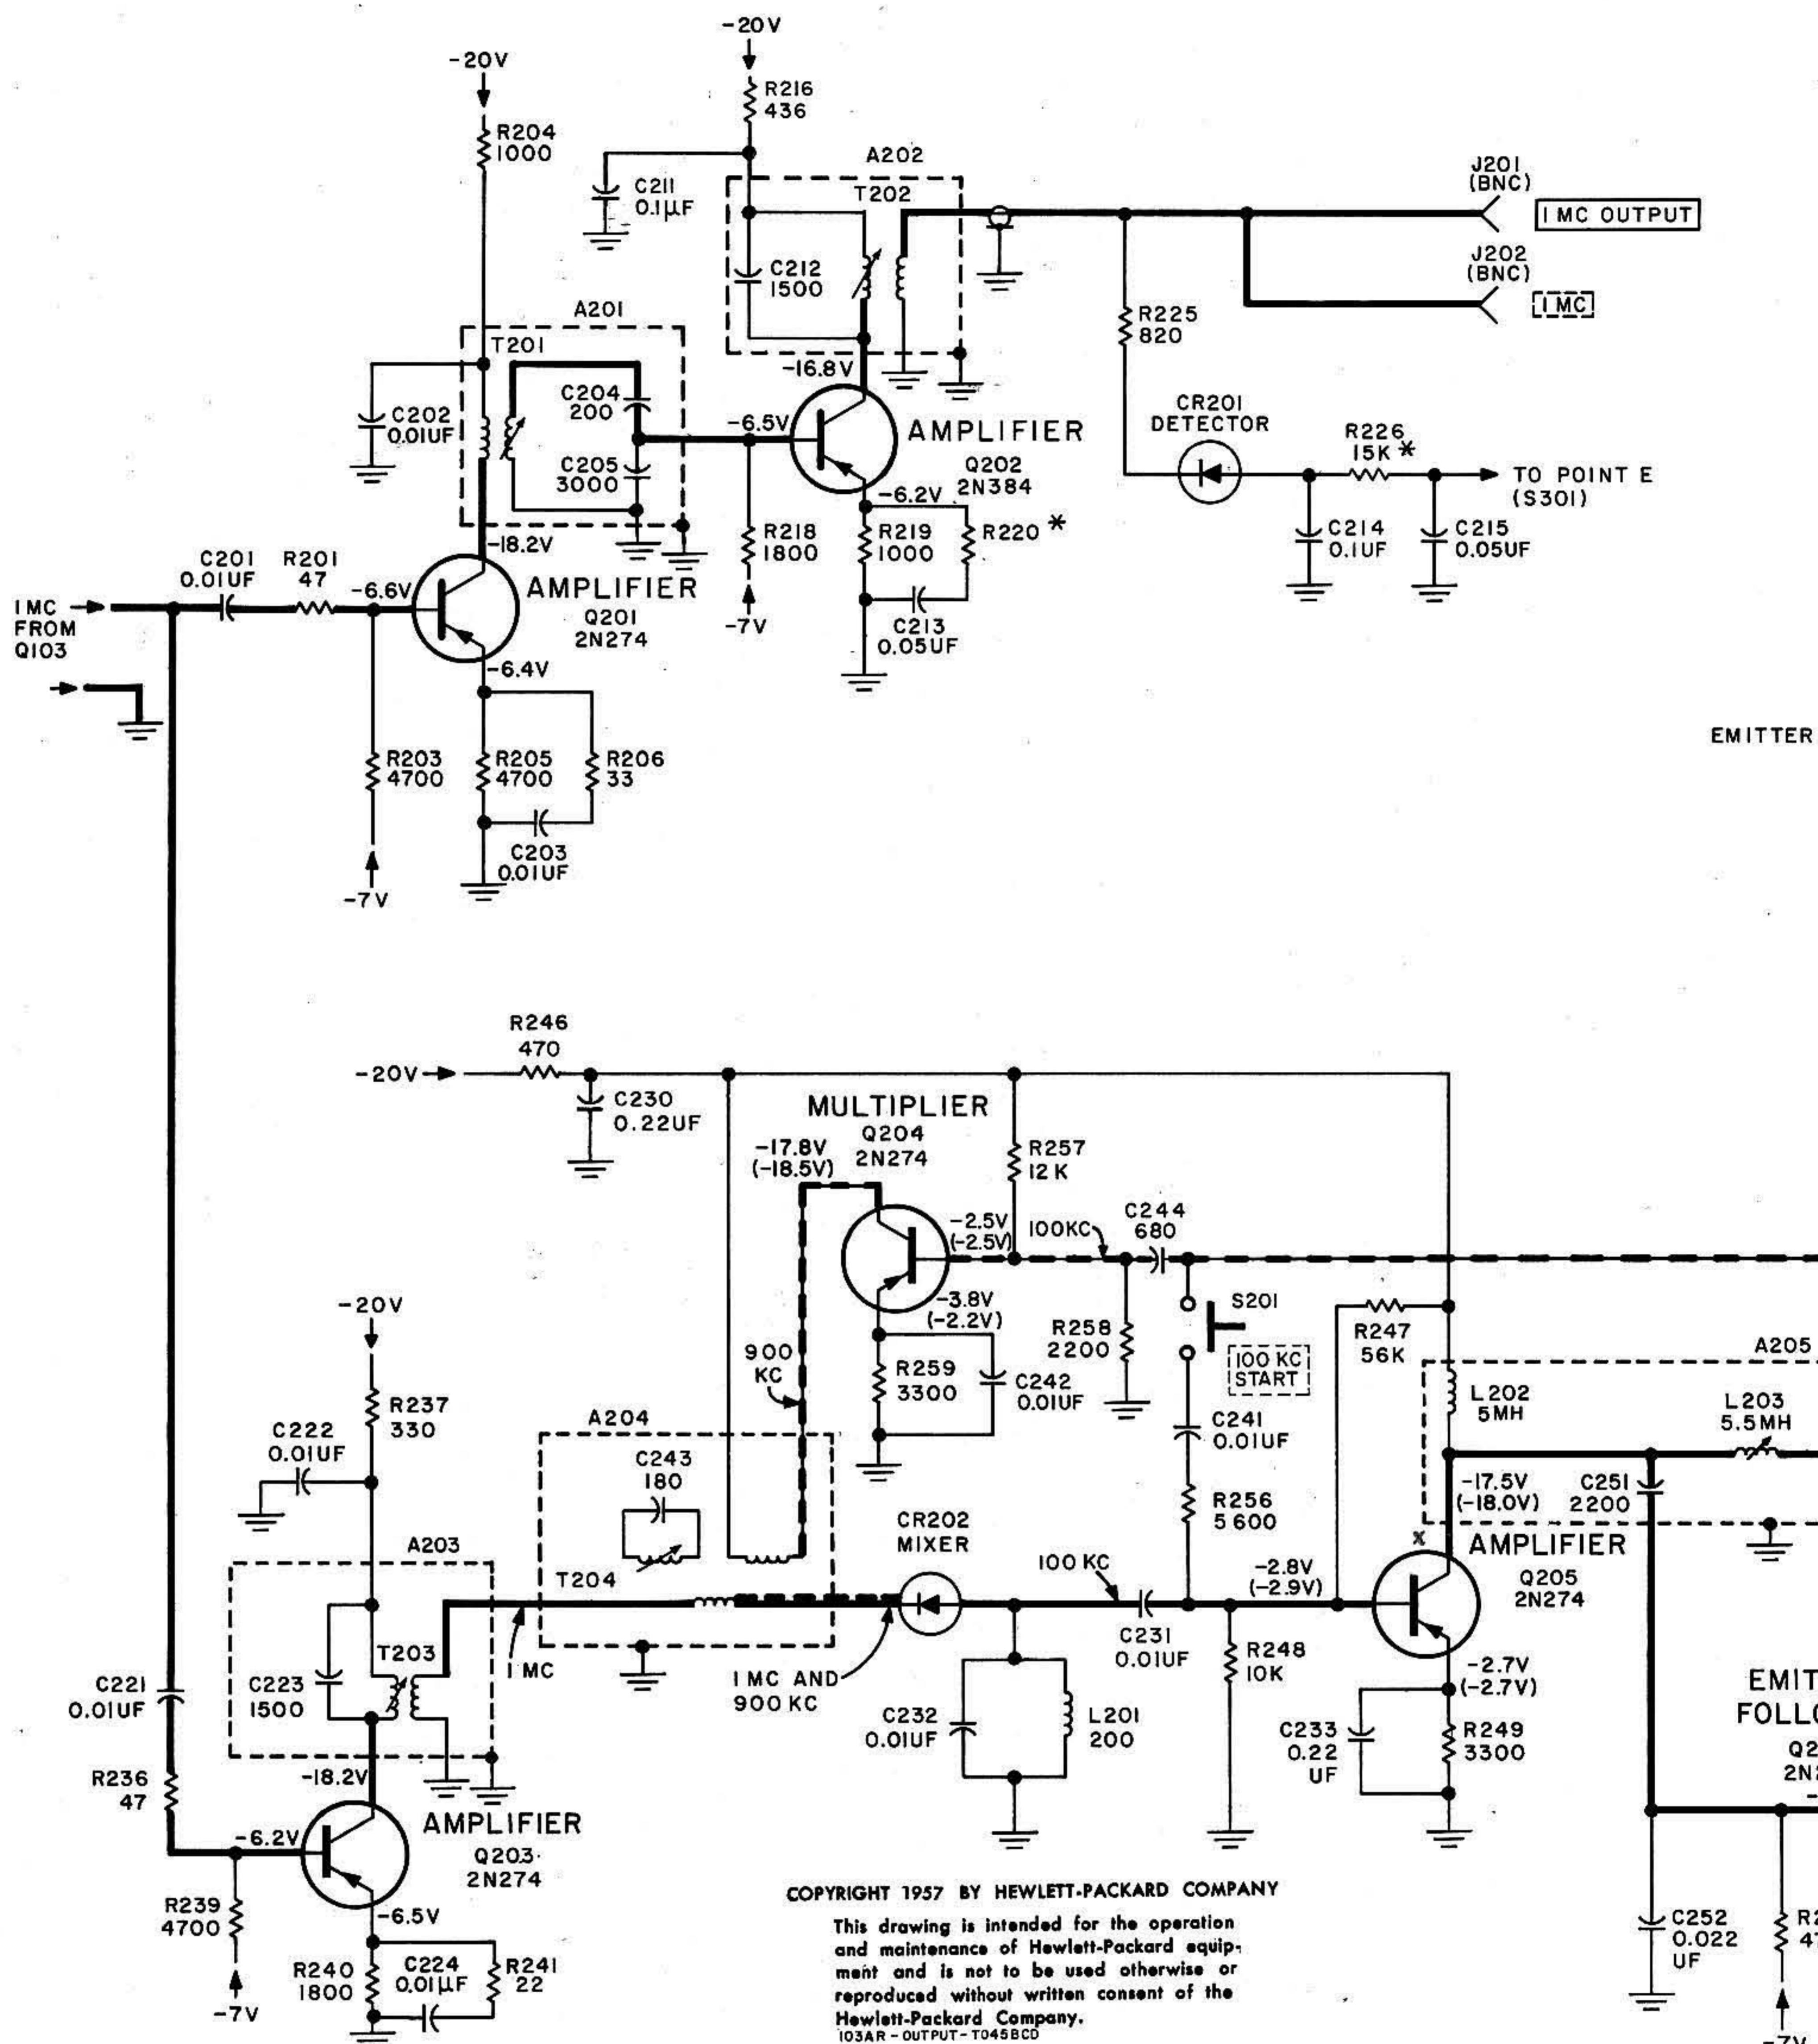

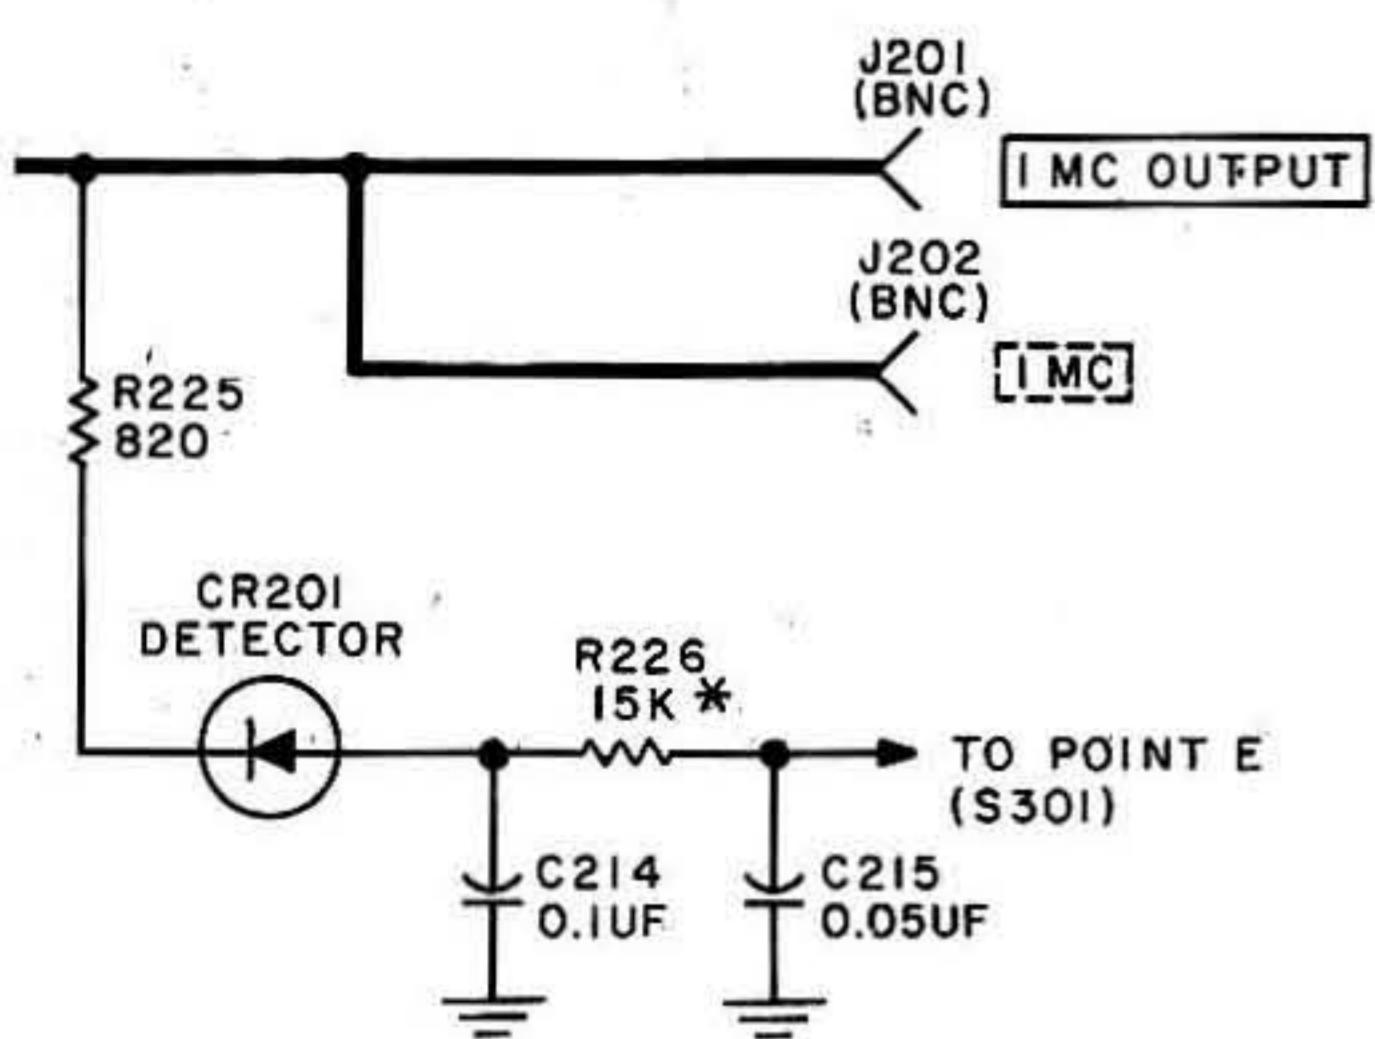

NOTES:

- 1) UNLESS OTHERWISE NOTED:
CAPACITY IN PF, RESISTANCE
IN OHMS, INDUCTANCE IN UH.
- 2) * SELECTED COMPONENT;
AVERAGE VALUE SHOWN.
- 3) ALL VOLTAGES $\pm 10\%$. VOLTAGES
IN PARENTHESES MEASURED WITH
REGENERATIVE DIVIDER NON-OPERATING.

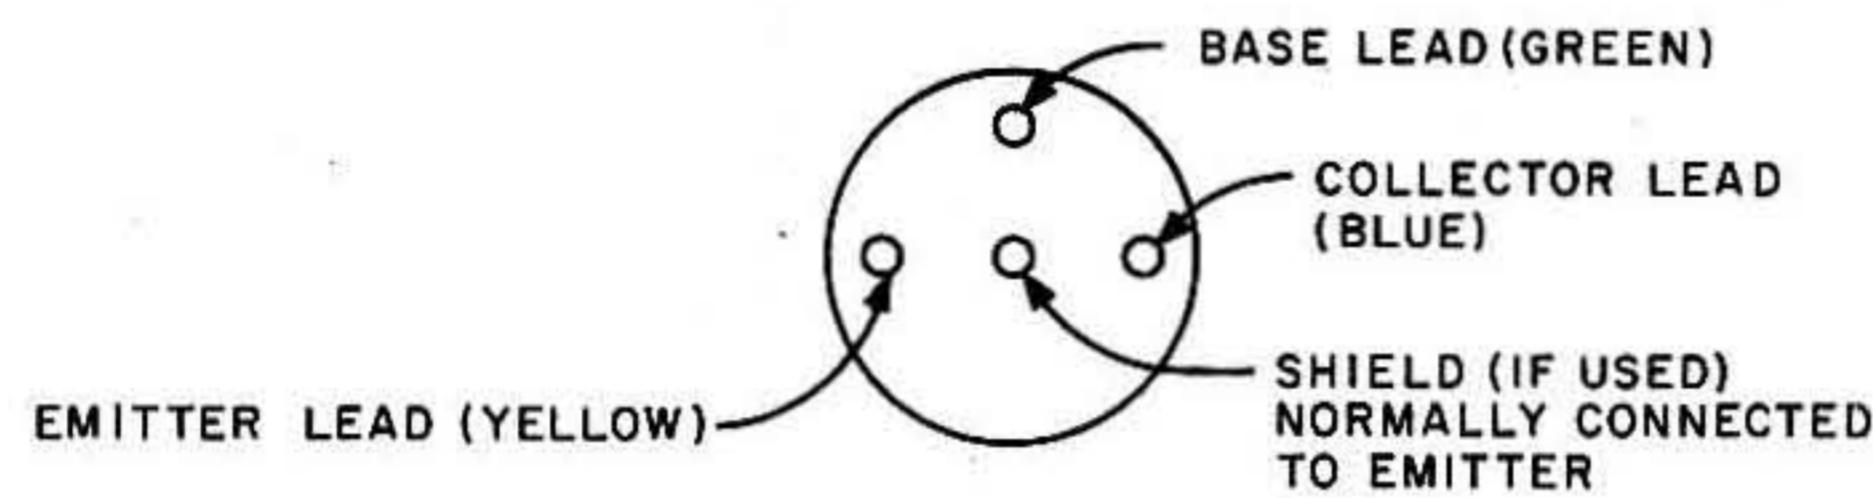

TRANSISTOR CONNECTIONS

REFERENCE DESIGNATORS

A201-206
C201-266
CR201-203
J201-205
L201-203
Q201-207
R201-287
S201
T201-205

OMITTED:

C206-210, 216-220,
225-229, 235-240,
245-250, 255-260.
R202, 207-215, 217, 221-224,
227-235, 238, 242-245,
250-255, 260-266, 271-
274, 276, 281-285

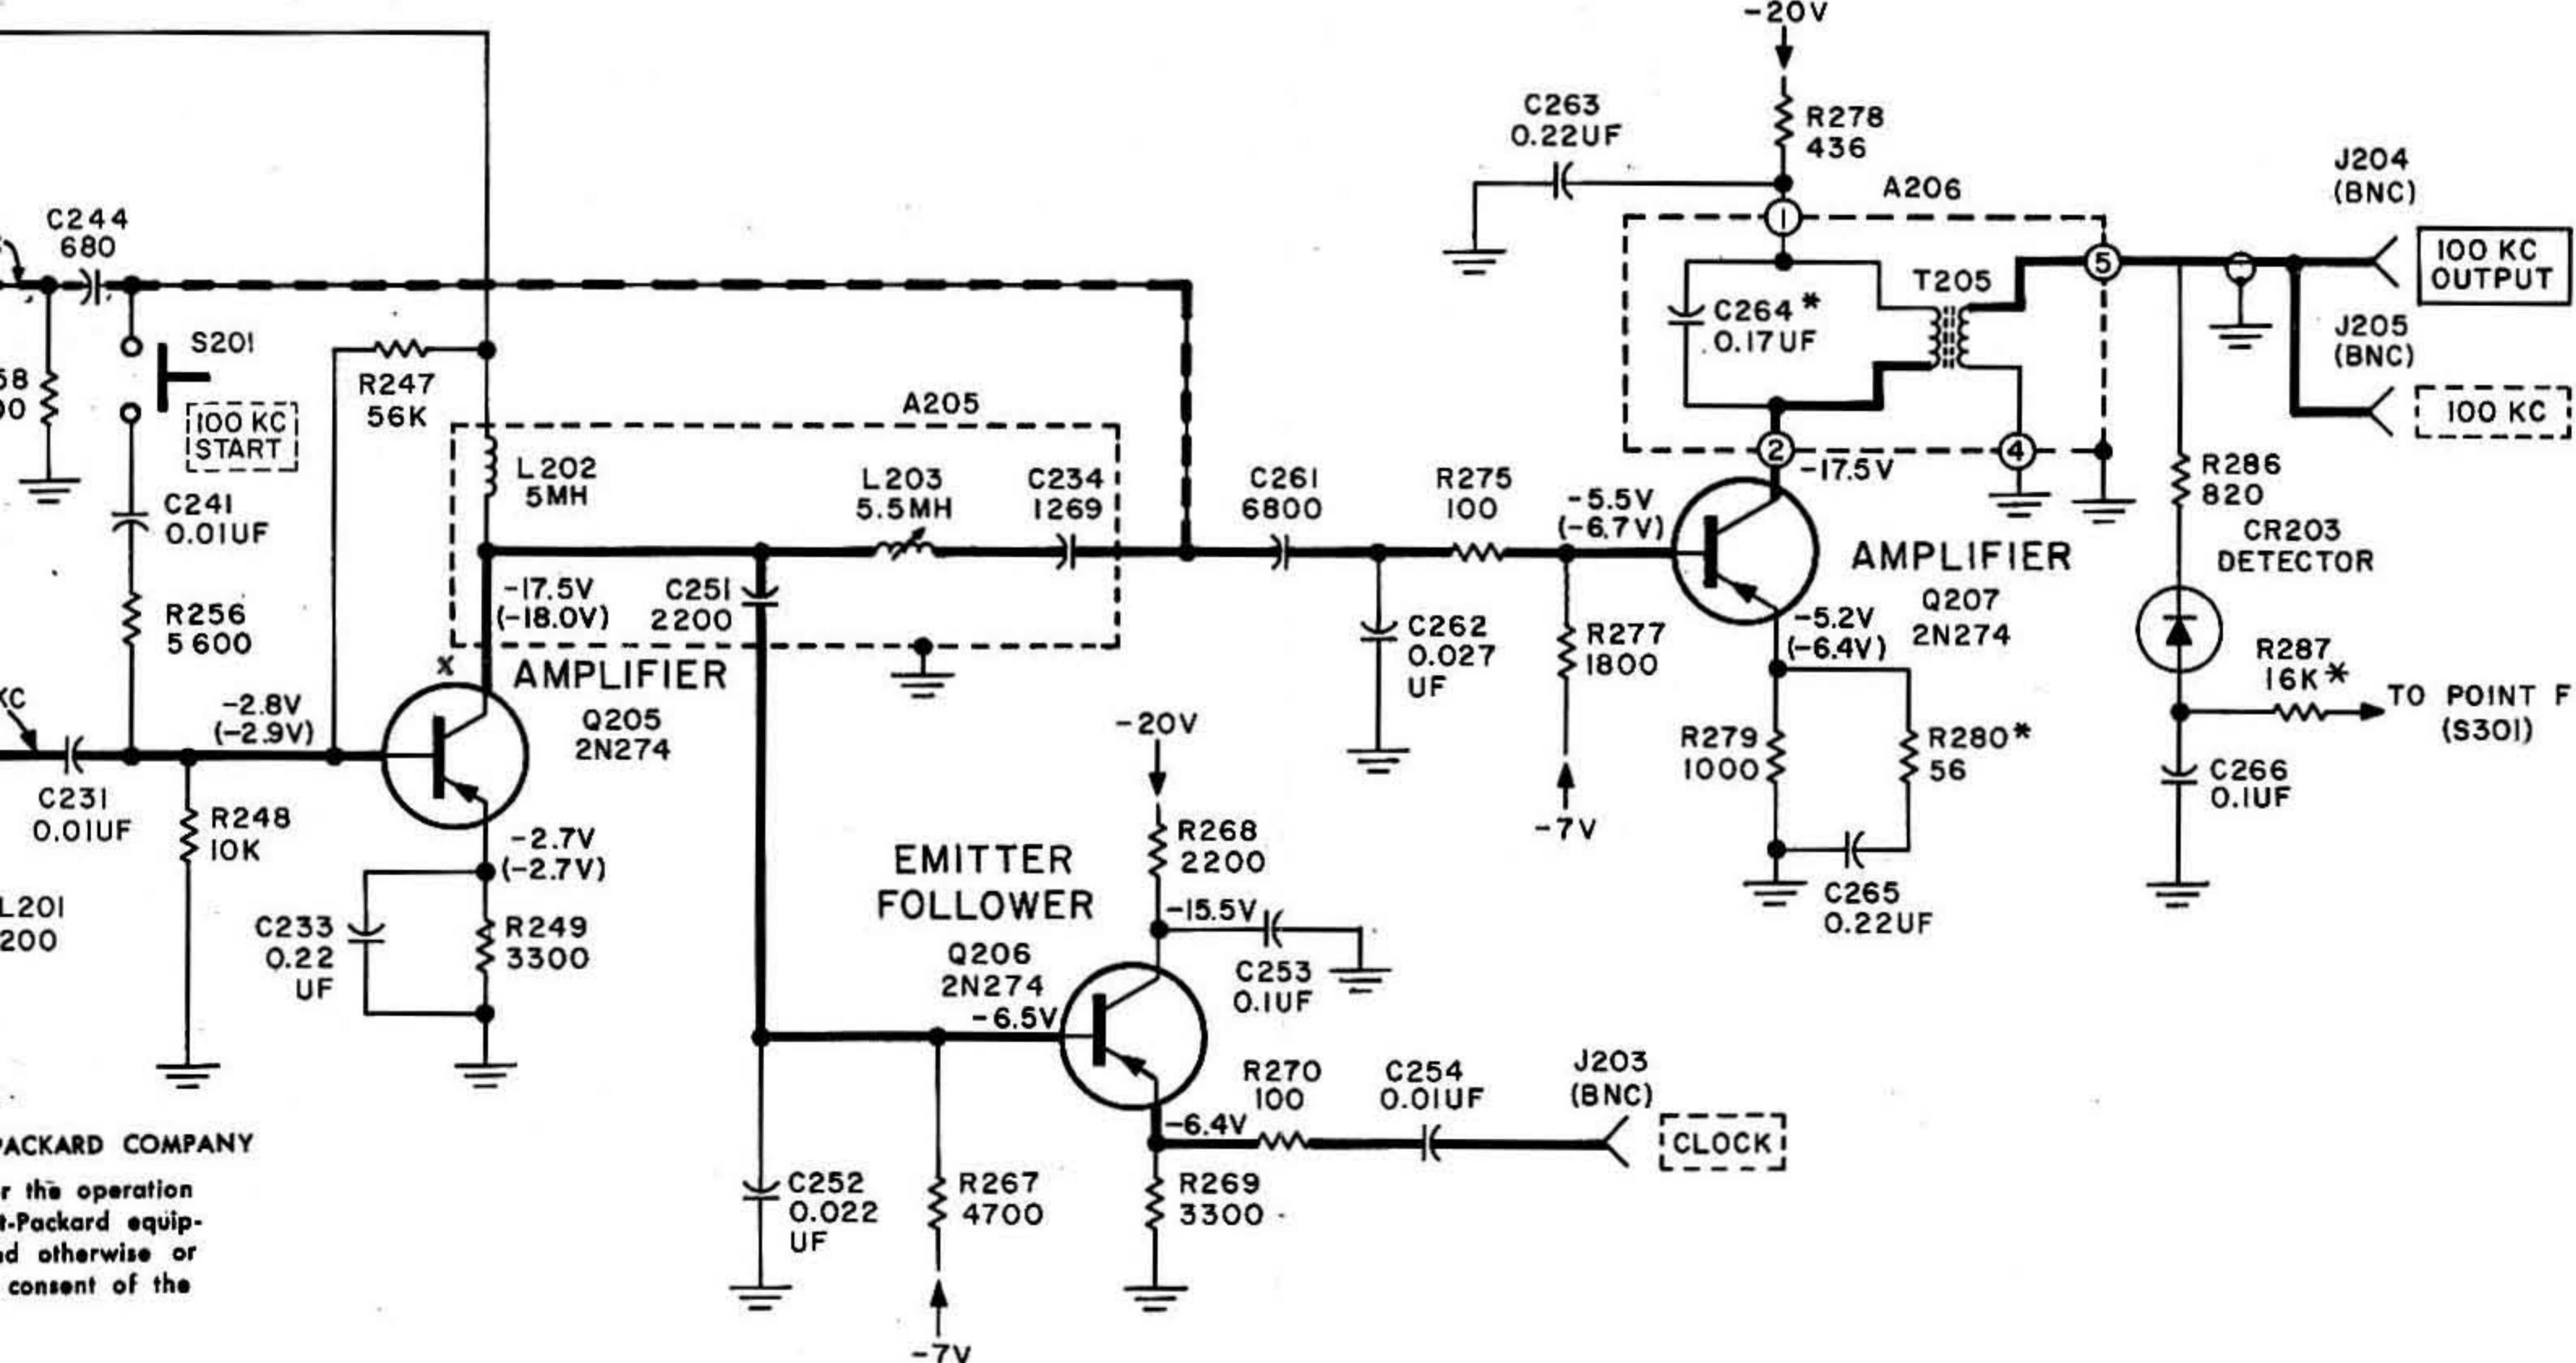
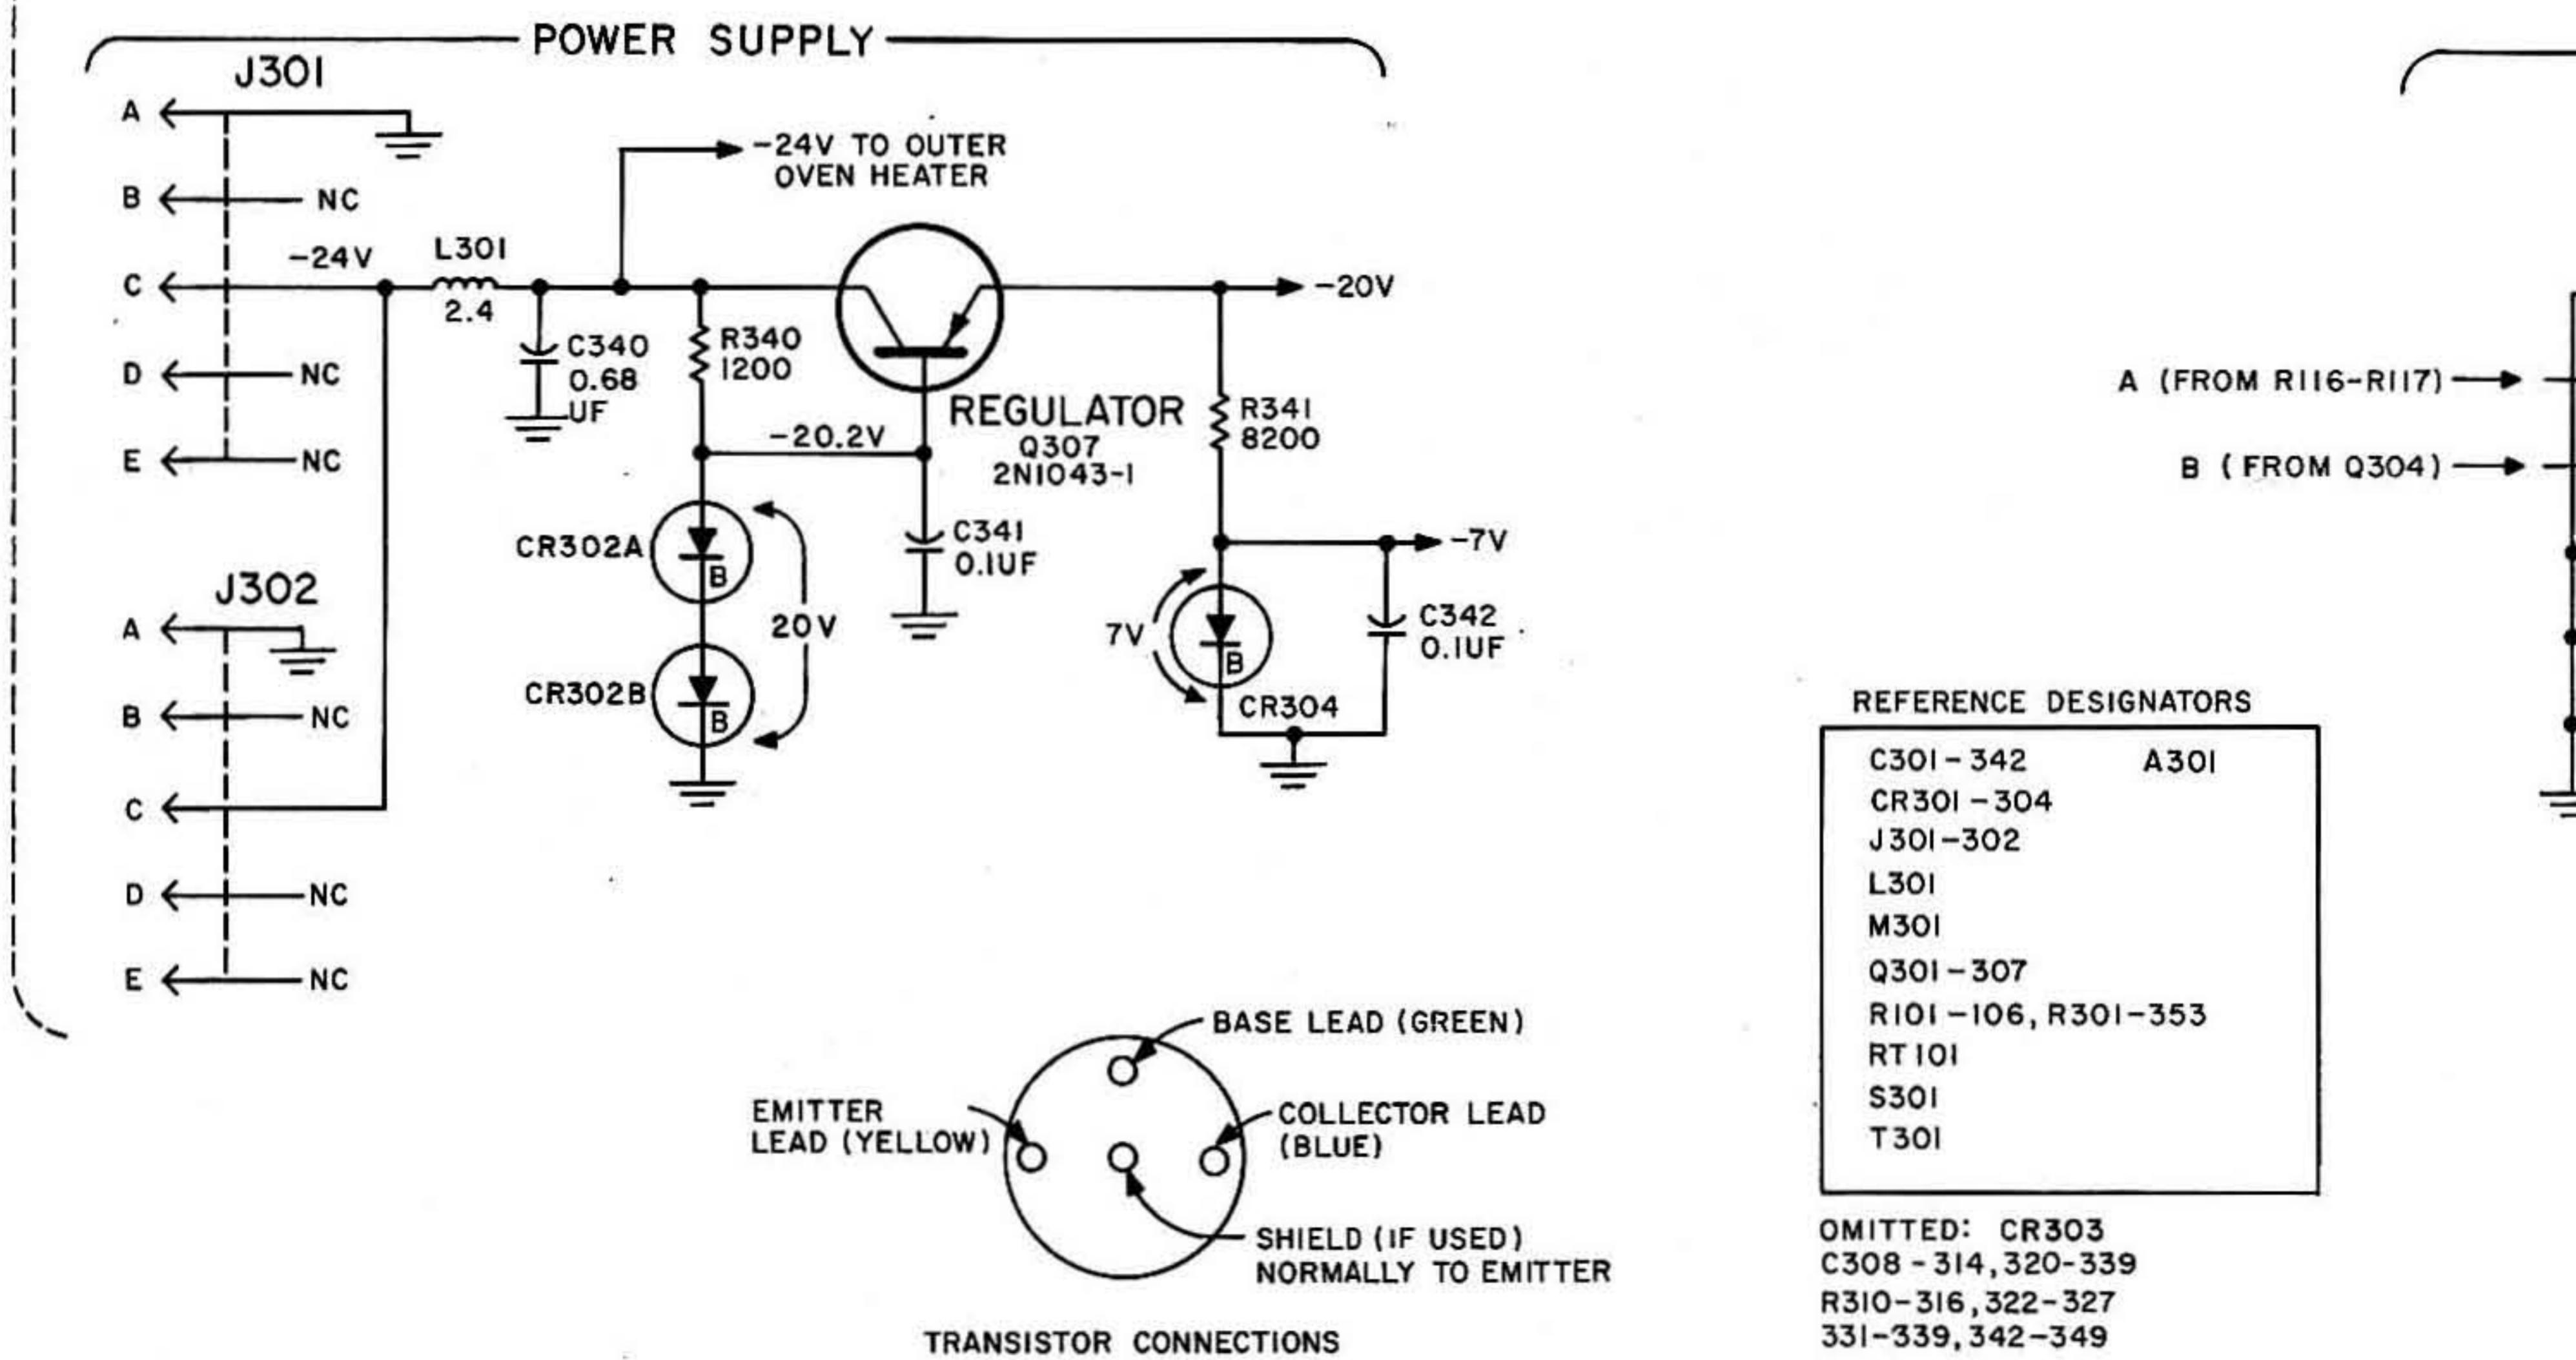
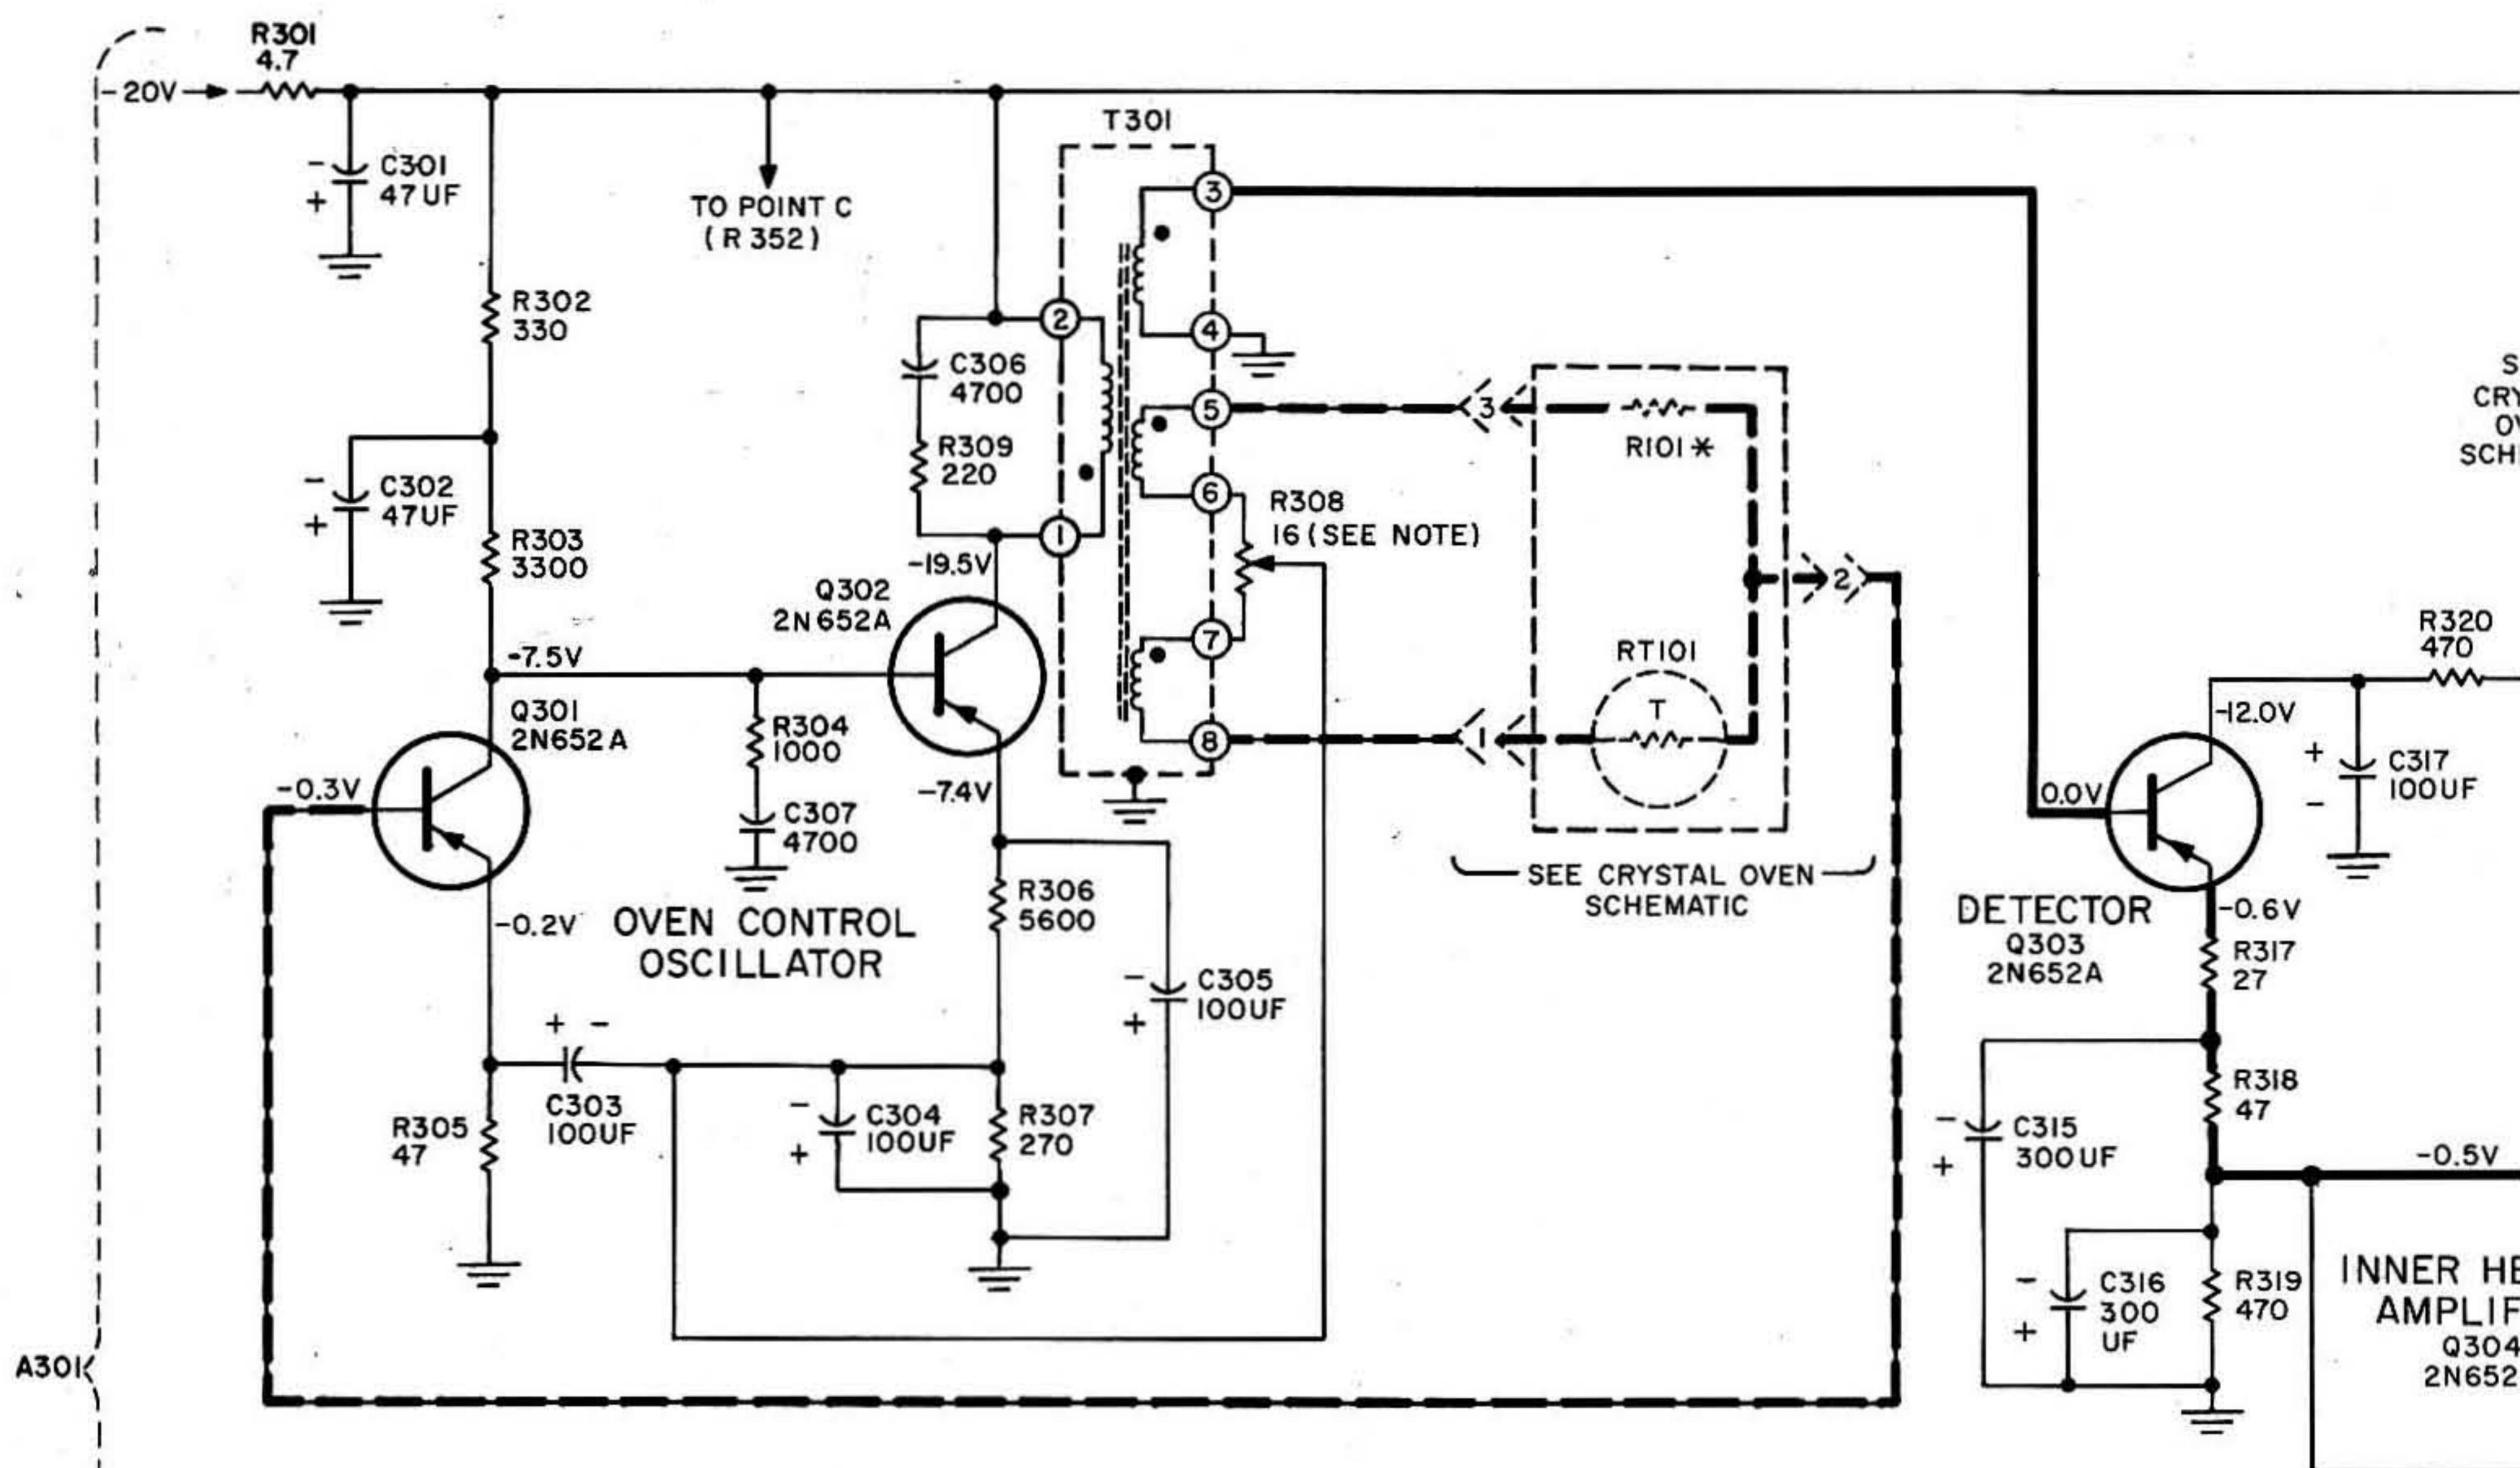


Figure 8-3. Output

Model 103AR



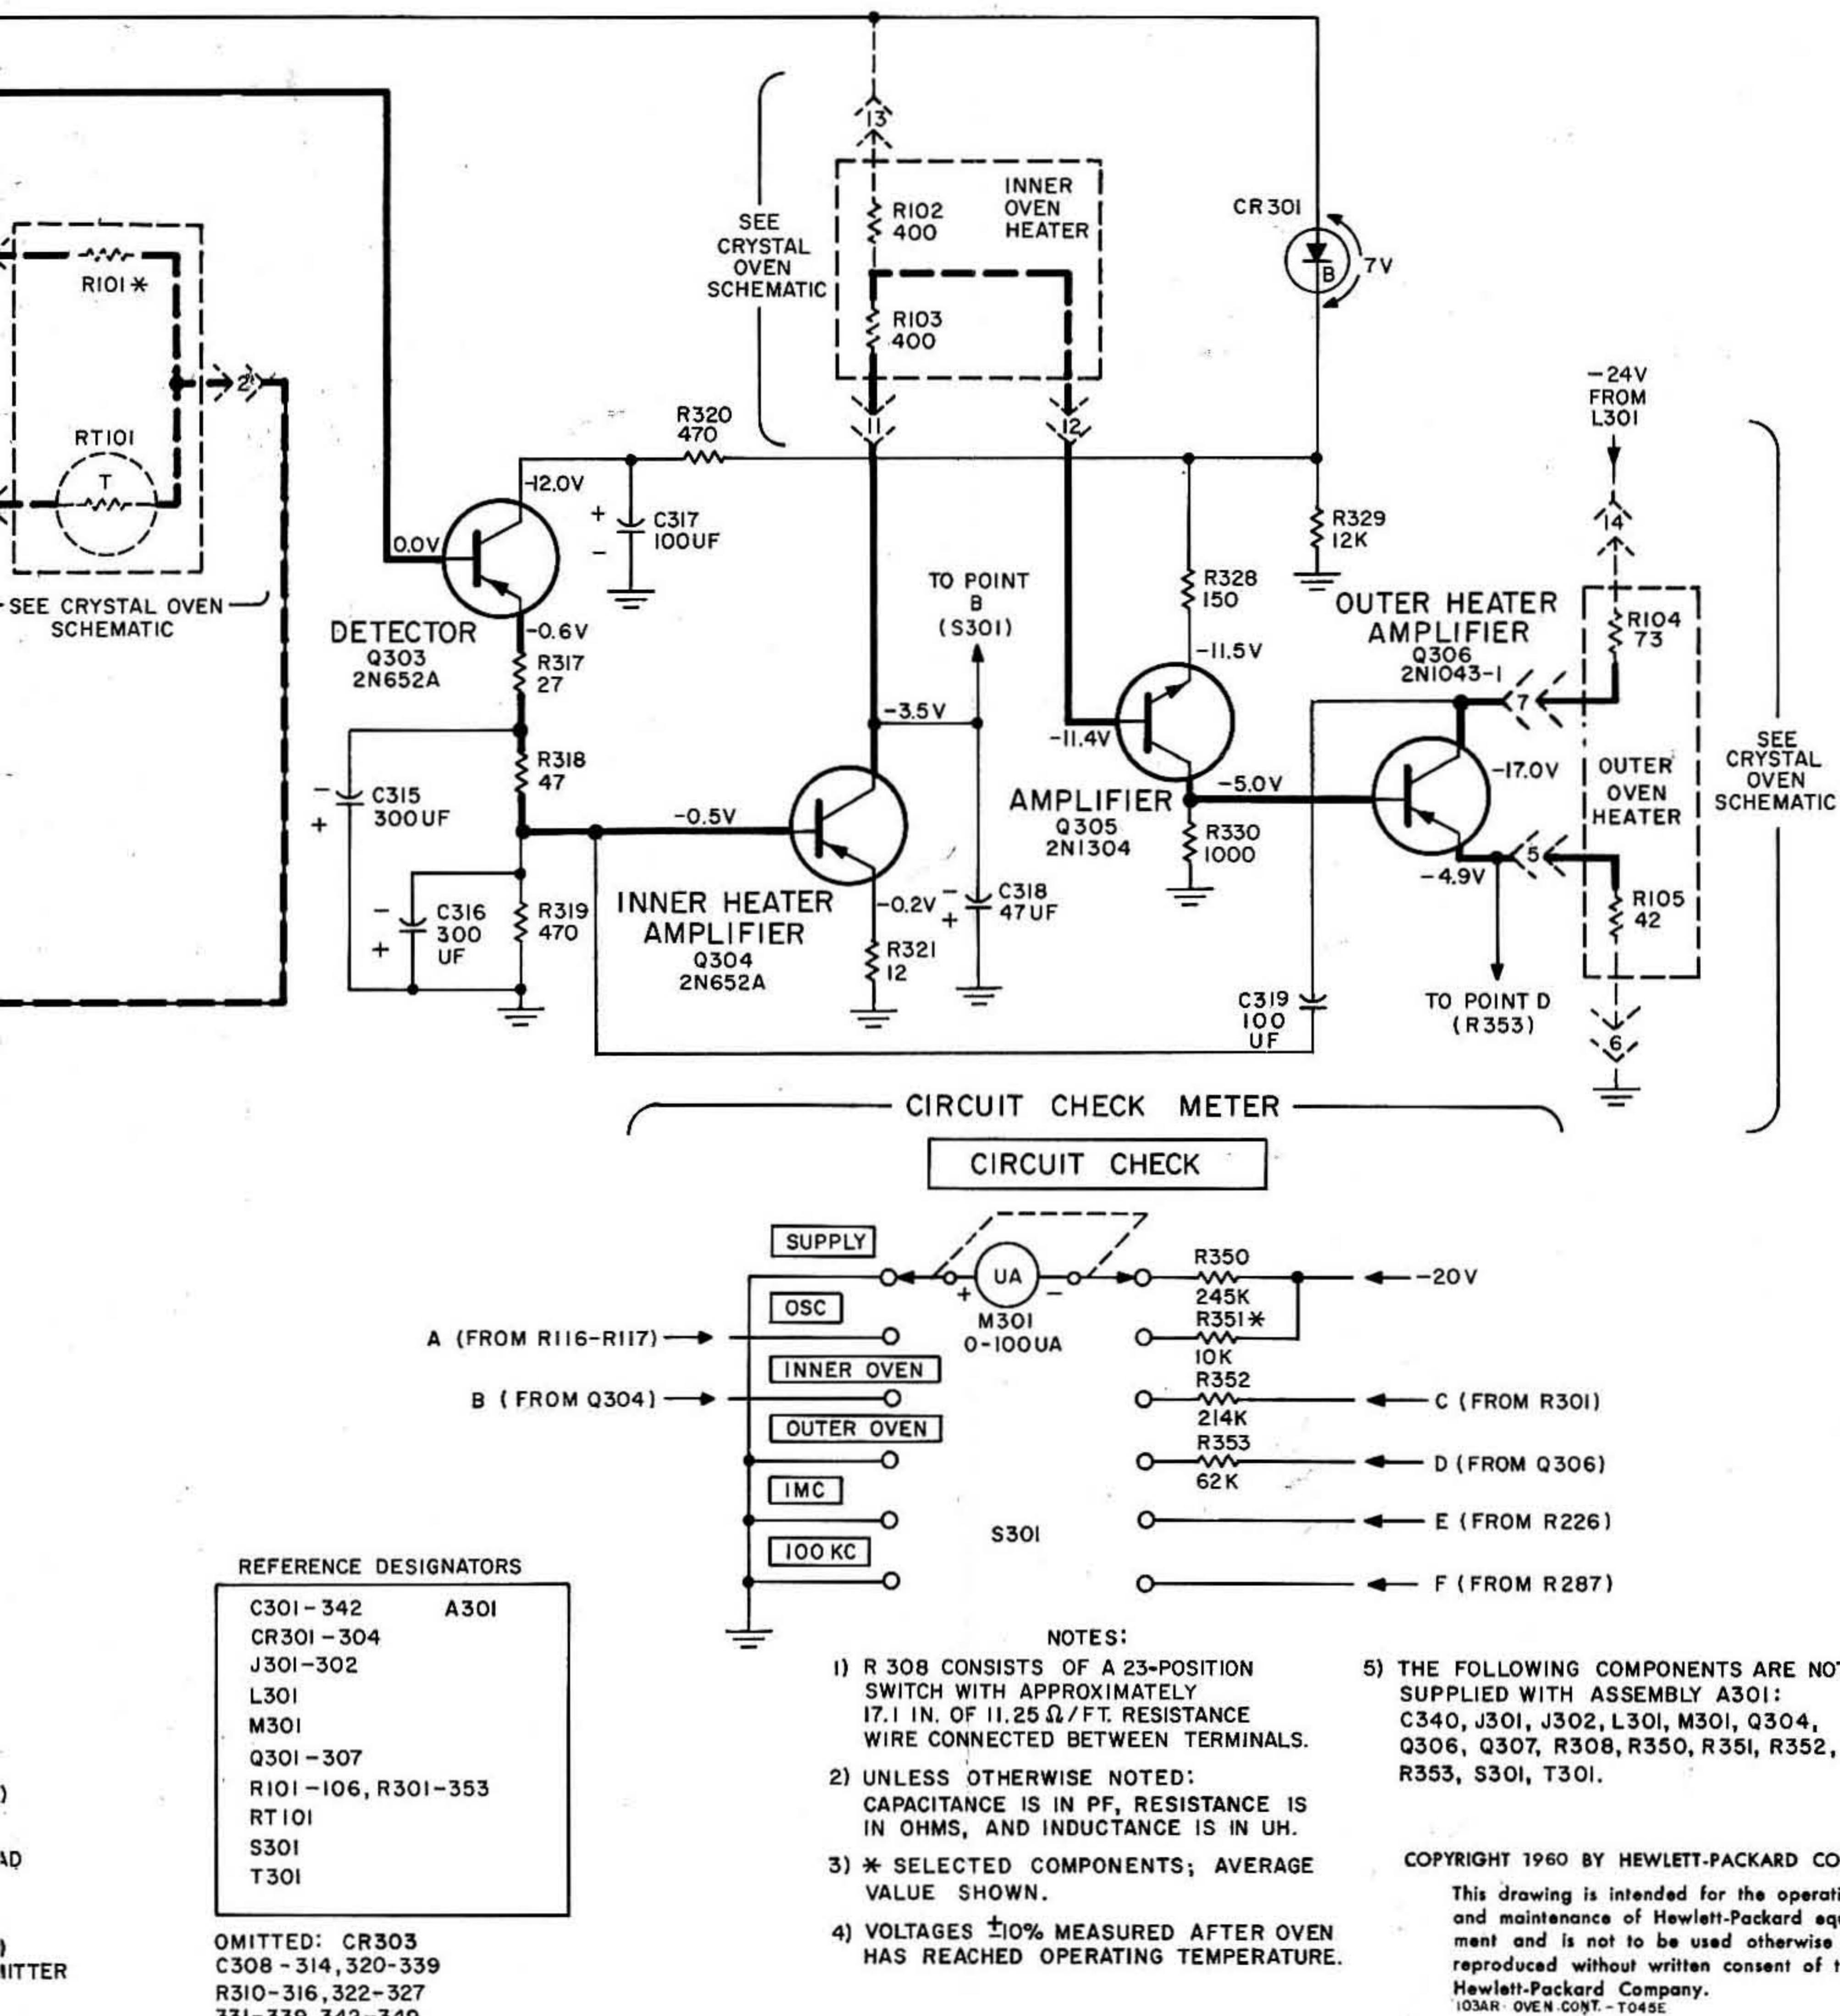


Figure 8-4. Oven Control